

## Technical Information

### Waterpilot FMX21

Hydrostatic level measurement

Compact device for level measurement in fresh water, wastewater and saltwater, communication via HART



Reliable and robust level probe with ceramic measuring cell

#### Application

The Waterpilot FMX21 is a pressure sensor for hydrostatic level measurement. Endress+Hauser offers three different versions of the FMX21 sensor:

- FMX21 with a stainless steel housing, outer diameter of 22 mm (0.87 in): Standard version suitable for drinking water applications and for use in bore holes and wells with small diameters.
- FMX21 with a stainless steel housing, outer diameter of 42 mm (1.65 in): Heavy duty version, easy clean flush-mounted process diaphragm. Ideally suited for wastewater and sewage treatment plants.
- FMX21 with a plastic insulation, outer diameter of 29 mm (1.14 in): Corrosion-resistant version generally for use in saltwater, particularly for ship ballast water tanks.

#### Your benefits

- High resistance to overload and aggressive media
- High-precision, robust ceramic measuring cell with long-term stability
- Climate proofed sensor thanks to completely potted electronics and 2-filter pressure compensation system
- 4 to 20 mA with superimposed HART 6.0 output signal
- Simultaneous measurement of level and temperature with optionally integrated Pt100 temperature sensor
- Accuracy
  - Reference accuracy  $\pm 0.2\%$
  - PLATINUM version  $\pm 0.1\%$
- Automatic density compensation to increase accuracy
- Usage in drinking water: KTW, NSF, ACS
- Approvals: ATEX, FM, CSA
- Marine certificate: GL, ABS, LR, BV, DNV
- Extensive range of accessories provides complete measuring point solutions



## Table of contents

|                                                                                   |    |                                                                                          |    |
|-----------------------------------------------------------------------------------|----|------------------------------------------------------------------------------------------|----|
| <b>Document information</b> .....                                                 | 3  | <b>Medium temperature limits</b> .....                                                   | 19 |
| Document conventions .....                                                        | 3  |                                                                                          |    |
| <b>Function and system design</b> .....                                           | 5  | <b>Mechanical construction</b> .....                                                     | 20 |
| Device selection .....                                                            | 5  | Dimensions of the level probe .....                                                      | 20 |
| Measuring principle .....                                                         | 6  | Dimensions of the mounting clamp .....                                                   | 20 |
| Measuring system .....                                                            | 7  | Dimensions of the extension cable mounting screws .....                                  | 21 |
| Level measurement with absolute pressure probe and external pressure signal ..... | 9  | Dimensions of the IP66, IP67 terminal boxes with filters .....                           | 21 |
| Density compensation with Pt100 temperature sensor .....                          | 9  | Dimensions of the TMT182 temperature head transmitter .....                              | 22 |
| Communication protocol .....                                                      | 10 | Terminal box with integrated TMT182 temperature head transmitter (4 to 20 mA HART) ..... | 22 |
| System integration .....                                                          | 10 | Weight .....                                                                             | 22 |
|                                                                                   |    | Material .....                                                                           | 23 |
| <b>Input</b> .....                                                                | 11 | Extension cable .....                                                                    | 25 |
| Measured variable .....                                                           | 11 | Terminals .....                                                                          | 25 |
| Measuring range .....                                                             | 11 |                                                                                          |    |
| Input signal .....                                                                | 11 | <b>Operability</b> .....                                                                 | 26 |
|                                                                                   |    | FieldCare .....                                                                          | 26 |
| <b>Output</b> .....                                                               | 12 | Field Xpert SFX .....                                                                    | 26 |
| Output signal .....                                                               | 12 |                                                                                          |    |
| Signal range .....                                                                | 12 | <b>Certificates and approvals</b> .....                                                  | 27 |
| Signal on alarm .....                                                             | 12 | CE mark .....                                                                            | 27 |
| Load .....                                                                        | 12 | Ex approval .....                                                                        | 27 |
| Damping .....                                                                     | 13 | Drinking water approval .....                                                            | 27 |
|                                                                                   |    | Marine certificate .....                                                                 | 27 |
| <b>Power supply</b> .....                                                         | 13 | Standards and guidelines .....                                                           | 27 |
| Supply voltage .....                                                              | 13 |                                                                                          |    |
| Power consumption .....                                                           | 13 | <b>Ordering information</b> .....                                                        | 28 |
| Current consumption .....                                                         | 13 | FMX21 .....                                                                              | 28 |
| Measuring unit electrical connection .....                                        | 13 | FMX21 (continued) .....                                                                  | 29 |
| Cable specifications .....                                                        | 15 |                                                                                          |    |
| Residual ripple .....                                                             | 15 | <b>Accessories</b> .....                                                                 | 30 |
|                                                                                   |    | Mounting clamp .....                                                                     | 30 |
| <b>Performance characteristics</b> .....                                          | 15 | Terminal box .....                                                                       | 30 |
| Reference operating conditions .....                                              | 15 | Additional weight .....                                                                  | 30 |
| Reference accuracy .....                                                          | 16 | TMT182 temperature head transmitter (4 to 20 mA HART) .....                              | 30 |
| Resolution .....                                                                  | 16 | Extension cable mounting screw .....                                                     | 30 |
| Long-term stability .....                                                         | 16 | Terminals .....                                                                          | 30 |
| Influence of medium temperature .....                                             | 16 | Cable shortening kit .....                                                               | 31 |
| Warm-up period .....                                                              | 16 | Cable marking .....                                                                      | 31 |
| Step response time .....                                                          | 16 | Testing adapter .....                                                                    | 31 |
|                                                                                   |    |                                                                                          |    |
| <b>Installation</b> .....                                                         | 17 | <b>Documentation</b> .....                                                               | 32 |
| Installation instructions .....                                                   | 17 | Field of activities .....                                                                | 32 |
| Additional installation instruction .....                                         | 17 | Technical Information .....                                                              | 32 |
|                                                                                   |    | Operating Instructions .....                                                             | 32 |
| <b>Environment</b> .....                                                          | 18 | Safety instructions .....                                                                | 32 |
| Ambient temperature range .....                                                   | 18 | Drinking water approval .....                                                            | 32 |
| Storage temperature range .....                                                   | 18 |                                                                                          |    |
| Degree of protection .....                                                        | 18 | <b>Patents</b> .....                                                                     | 32 |
| Geometric height according to IEC61010-1 Ed.3 .....                               | 18 |                                                                                          |    |
| Electromagnetic compatibility (EMC) .....                                         | 18 | <b>Configuration data sheet</b> .....                                                    | 33 |
| Overvoltage protection .....                                                      | 19 | Level .....                                                                              | 33 |
|                                                                                   |    | Pressure .....                                                                           | 33 |
| <b>Process</b> .....                                                              | 19 |                                                                                          |    |
| Medium temperature range .....                                                    | 19 |                                                                                          |    |

## Document information

### Document conventions

### Safety symbols

| Symbol                                                                                           | Meaning                                                                                                                                    |
|--------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------|
| <br>A0011189-09 | <b>DANGER!</b><br>This symbol alerts you to a dangerous situation. Failure to avoid this situation will result in serious or fatal injury. |
| <br>A0011190-09 | <b>WARNING!</b><br>This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in serious or fatal injury. |
| <br>A0011191-09 | <b>CAUTION!</b><br>This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or medium injury.  |
| <br>A0011192-09 | <b>NOTICE!</b><br>This symbol contains information on procedures and other facts which do not result in personal injury.                   |

### Electrical symbols

| Symbol                                                                                             | Meaning                                                                                                                                                                                                                                          |
|----------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <br>A0011193-01   | <b>Direct current</b><br>A terminal to which DC voltage is applied or through which direct current flows.                                                                                                                                        |
| <br>A0011194-01   | <b>Alternating current</b><br>A terminal to which alternating voltage is applied or through which alternating current flows.                                                                                                                     |
| <br>A0011195-01 | <b>Direct current and alternating current</b> <ul style="list-style-type: none"> <li>A terminal to which alternating voltage or DC voltage is applied.</li> <li>A terminal through which alternating current or direct current flows.</li> </ul> |
| <br>A0011196-01 | <b>Ground connection</b><br>A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.                                                                                                                  |
| <br>A0011197-01 | <b>Protective ground connection</b><br>A terminal which must be connected to ground prior to establishing any other connections.                                                                                                                 |
| <br>A0011198-01 | <b>Equipotential connection</b><br>A connection that has to be connected to the plant grounding system. This may be a potential equalization line or a star grounding system depending on national or company codes of practice.                 |

### Symbols for certain types of information

| Symbol                                                                                             | Meaning                                                              |
|----------------------------------------------------------------------------------------------------|----------------------------------------------------------------------|
| <br>A0011199-01 | <b>Tip</b><br>Indicates additional information.                      |
| <br>A0011200-01 | <b>Reference to page</b><br>Refers to the corresponding page number. |

### Symbols in graphics

| Symbol          | Meaning      |
|-----------------|--------------|
| 1, 2, 3, 4, ... | Item numbers |
| A, B, C, D, ... | Views        |

|                                                                                                                |                                                                              |
|----------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------|
| <br><small>ANSI Z39.1</small> | <b>Hazardous area</b><br>Indicates a hazardous area.                         |
| <br><small>ANSI Z39.1</small> | <b>Safe area (non-hazardous area)</b><br>Indicates a non-hazardous location. |

#### Symbols at the device

| Symbol                                                                            | Meaning                                                                                                                                                           |
|-----------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|  | <b>Connecting cable immunity to temperature change</b><br>Indicates that the connecting cables must be able to withstand temperatures of at least 85 °C (185 °F). |

## Function and system design

### Device selection


|                           |                                                                                                                                                                                                                                                                                                                                                                                                                                |                                                                                    |                                                                                     |
|---------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|
| Waterpilot FMX21          |                                                                                                                                                                                                                                                                                                                                               |  |  |
| Field of application      | Hydrostatic level measurement in deep wells e.g. drinking water                                                                                                                                                                                                                                                                                                                                                                | Hydrostatic level measurement in wastewater                                        | Hydrostatic level measurement in saltwater                                          |
|                           | <b>NOTICE</b><br>The Waterpilot is not suitable for use in biogas plants since the gases can diffuse through the elastomers (seals, extension cable).<br>• For applications with biogas Endress+Hauser offers the level transmitter Deltapilot.                                                                                                                                                                                |                                                                                    |                                                                                     |
| Process connection        | ▪ Mounting clamp<br>▪ Extension cable mounting screw with G 1/4" A or NPT 1/4" thread                                                                                                                                                                                                                                                                                                                                          |                                                                                    |                                                                                     |
| Outer diameter            | 22 mm (0.87 in)                                                                                                                                                                                                                                                                                                                                                                                                                | 42 mm (1.65 in)                                                                    | max. 29 mm (1.14 in)                                                                |
| Extension cable           | PE, PUR, FEP (→ 1/25)                                                                                                                                                                                                                                                                                                                                                                                                          |                                                                                    |                                                                                     |
| Seals                     | ▪ FKM Viton<br>▪ EPDM <sup>1)</sup>                                                                                                                                                                                                                                                                                                                                                                                            | FKM Viton                                                                          | ▪ FKM Viton<br>▪ EPDM <sup>1)</sup>                                                 |
| Measuring ranges          | ▪ Gauge pressure: from 0 to 0.1 bar to 0 to 20 bar (0 to 1.5 psi to 0 to 300 psi)<br>▪ Absolute pressure: from 0 to 2 bar to 0 to 20 bar (0 to 30 psi to 0 to 300 psi)<br><br>▪ Customer-specific measuring ranges; factory-calibrated<br>▪ The following output units can be configured: %, mbar, bar, kPa, MPa, mmH <sub>2</sub> O, mH <sub>2</sub> O, inH <sub>2</sub> O, ftH <sub>2</sub> O, psi and numerous level units. |                                                                                    |                                                                                     |
| Overload                  | Up to 40 bar (600 psi)                                                                                                                                                                                                                                                                                                                                                                                                         |                                                                                    | Up to 25 bar (375 psi)                                                              |
| Process temperature range | -10 to +70 °C (+14 to +158 °F)                                                                                                                                                                                                                                                                                                                                                                                                 |                                                                                    | 0 to +50 °C (+32 to +122 °F)                                                        |
| Reference accuracy        | ▪ ±0.2 % of the set span<br>▪ Optional: ±0.1 % of set span (PLATINUM version)                                                                                                                                                                                                                                                                                                                                                  |                                                                                    |                                                                                     |
| Supply voltage            | 10.5 to 35 V DC, Ex: 10.5 to 30 V DC                                                                                                                                                                                                                                                                                                                                                                                           |                                                                                    |                                                                                     |
| Output                    | 4 to 20 mA (invertible) with superimposed digital communication protocol HART 6.0, 2-wire                                                                                                                                                                                                                                                                                                                                      |                                                                                    |                                                                                     |
| Options                   | Drinking water approval                                                                                                                                                                                                                                                                                                                                                                                                        | —                                                                                  |                                                                                     |
|                           | ▪ Large selection of approvals, including ATEX, FM, CSA<br>▪ Broad range of accessories<br>▪ Integrated Pt100 temperature sensor and TMT182 temperature head transmitter (4 to 20 mA HART)<br>▪ Marine certificate                                                                                                                                                                                                             |                                                                                    |                                                                                     |
| Specialties               | ▪ High-precision, robust ceramic measuring cell with long-term stability<br>▪ Automatic density compensation<br>▪ Customer specific cable marking<br>▪ Absolute pressure measuring cell                                                                                                                                                                                                                                        |                                                                                    |                                                                                     |

1) Recommended for drinking water applications and not for use in hazardous areas.



### Measuring principle

The ceramic measuring cell is a dry measuring cell, i.e. pressure acts directly on the robust ceramic process isolating diaphragm of the Waterpilot FMX21. Any changes in the air pressure are routed through the extension cable, via a pressure compensation tube, to the rear of the ceramic process isolating diaphragm and compensated for. A pressure-dependent change in capacitance caused by the movement of the process isolating diaphragm is measured at the electrodes of the ceramic carrier. The electronics then convert this into a signal which is proportional to the pressure and is linear to the level of the medium.

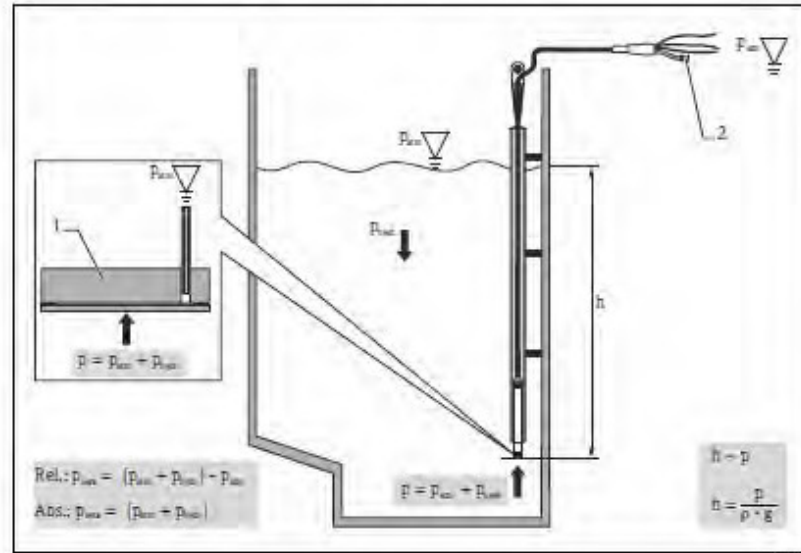

### Temperature measurement with optional Pt100 resistance thermometer <sup>1)</sup>

Endress+Hauser also offers the Waterpilot FMX21 with an optional 4-wire Pt100 resistance thermometer to measure level and temperature simultaneously (→ 30). The Pt100 belongs to Accuracy Class B in accordance with DIN EN 60751.

### Temperature measurement with optional Pt100 and TMT182 temperature head transmitter <sup>1)</sup>

Endress+Hauser also offers the TMT182 temperature head transmitter with the HART protocol to convert the temperature signal to an analog, scalable 4 to 20 mA output signal superimposed with HART 6.0.


See also: 'Density compensation with Pt100 temperature sensor' (→ 9); 'Ordering information' (→ 38); 'Accessories' (→ 30) and Technical Information TI00078R.

1) Not for use in hazardous areas.

### Measuring system

As standard, the complete measuring system consists of a Waterpilot FMX21 and a transmitter power supply unit with a supply voltage of 10.5 to 30 V DC (hazardous areas) or 10.5 to 35 V DC (non-hazardous areas).


Possible measuring point solutions with a transmitter and evaluation units from Endress+Hauser:

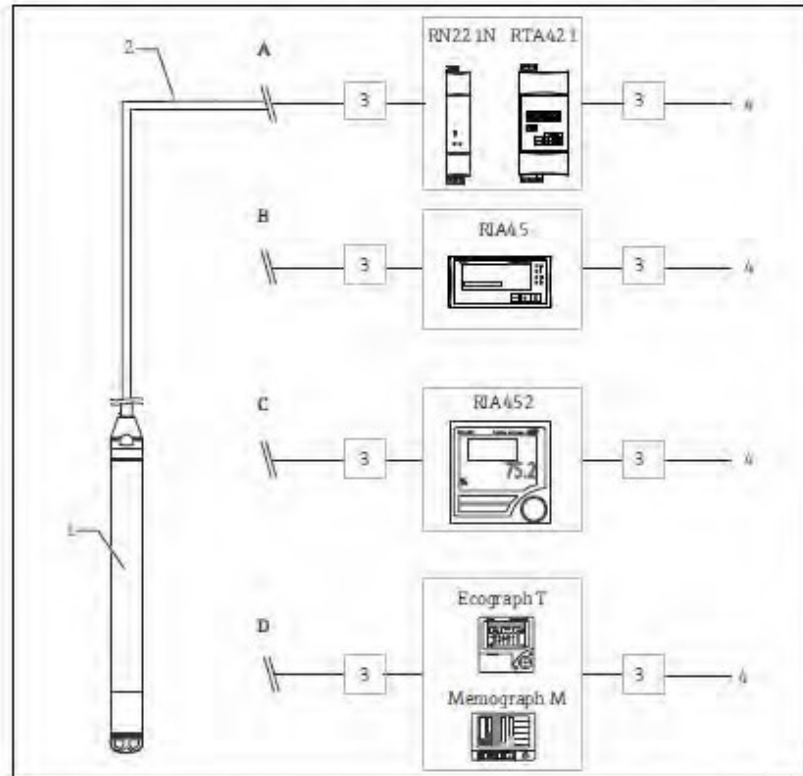

#### Application examples

- 1 Waterpilot FMX21 HART
- 2 4 to 20 mA HART
- 3 Overvoltage protection (OP), e.g. HAW from Endress+Hauser (not for use in hazardous areas)  
- OP on the sensor side for field installation: HAW569; for top-hat rail/DIN rail: HAW562/Intrinsically safe HAW5622  
- OP on the supply side for top-hat rail/DIN rail: HAW561 (115/230 V) and HAW561K (24/48 V AC/DC)
- 4 The overvoltage protection selected must be appropriate for the supply voltage.  
Power supply

- A Simple cost-effective measuring point solution: Power supply of Waterpilot in hazardous and non-hazardous areas using RN22 1N active barrier. Power supply and additional control of two consumers, e.g. pumps, via limit switch RTA42 1 with onsite display.
- B Evaluation unit RIA4 5 (for panel mounting) provides a power supply system, an onsite display and two switch outputs.
- C If several pumps are used, the pump service life can be prolonged by alternate switching. With alternating pump control, the pump which was out of service for the longest period of time is switched on. The evaluation unit RIA452 (for panel mounting) provides this option in addition to several other functions.
- D State-of-the-art recording technology with graphic display recorders from Endress+Hauser, such as Ecograph T, Memograph M, or paper recorders such as Alphalog for documenting, monitoring, visualizing and archiving purposes.

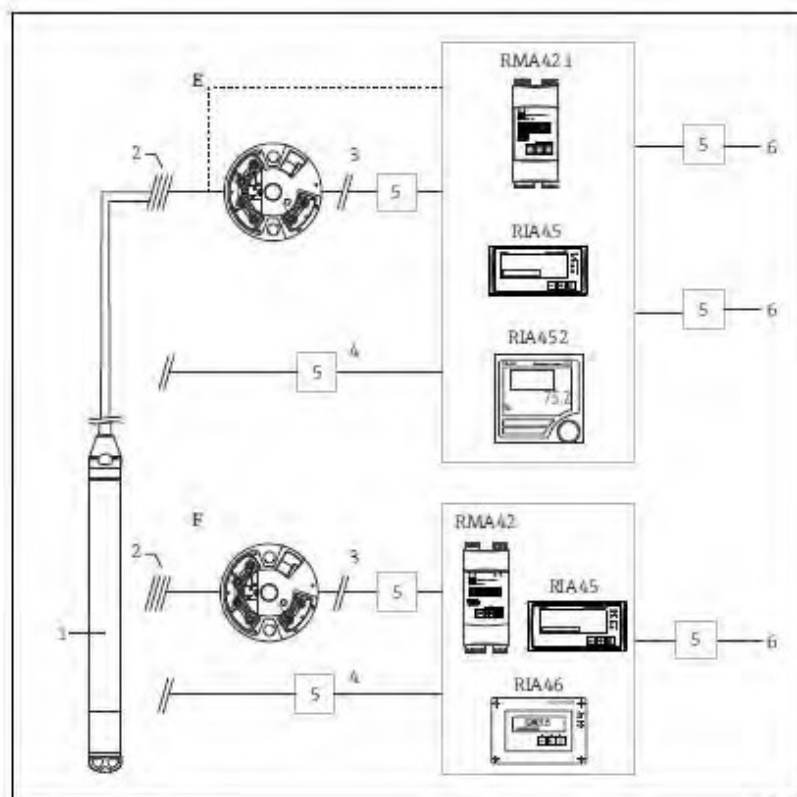

Application examples with Pt100

- 1 Waterpilot FMX21 HART  
 2 Connection for integrated Pt100 temperature sensor in the FMX21  
 3 4 to 20 mA HART (Temperature)  
 4 4 to 20 mA HART (Level)  
 5 Overvoltage protection (OP), e.g. HAW from Endress+Hauser (not for use in hazardous areas)  
 - OP on the sensor side for field installation: HAW569; for top-hat rail/DINrail: HAW562/intrinsically safe HAW562Z  
 - OP on the supply side for top-hat rail/DINrail: HAW563 (11.5/230 V) and HAW561K (24/48 V AC/DC)  
 The overvoltage protection selected must be appropriate for the supply voltage.  
 6 Power supply


**E** If you want to measure, display and evaluate the temperature as well as the level, e.g. to monitor temperature in fresh water to detect temperature limits for germ formation, you have the following options:

The optional TMT182 temperature head transmitter can convert the Pt100 signal to a 4 to 20 mA HART signal and transfer it to any common evaluation unit. The RMA421, RIA45 and RIA452 evaluation units also offer a direct input for the Pt100 signal.

**F** If you want to record and evaluate the level and temperature measured value with one device, use the RMA42, RIA45 and RIA46 evaluation units with two inputs. It is even possible to mathematically link the input signals with this unit. These evaluation units are not HART-compatible.



### Level measurement with absolute pressure probe and external pressure signal

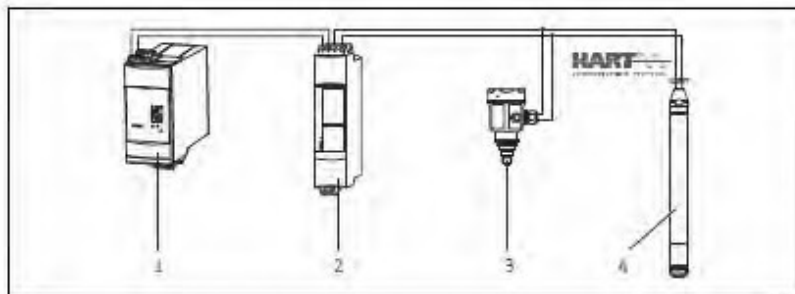

- 1 Fieldgate FK4520
- 2 Multidrop-Connector FXN520
- 3 Cerabar
- 4 Waterpilot FMX21

It is advisable to use an absolute pressure probe for applications in which condensation can occur. In the case of level measurement with an absolute pressure probe, the measured value is affected by fluctuations in the ambient pressure. To correct the resulting measured error, you can connect an external absolute pressure sensor (e.g. Cerabar) to the HART signal cable, switch the waterpilot to the burst mode and the Cerabar to operate in mode "Electr. Delta P". The external absolute pressure sensor then calculates the difference between the two pressure signals and can thus determine the level precisely. Only one level measured value can be corrected in this way.



If using intrinsically safe devices, strict compliance with the rules for interconnecting intrinsically safe circuits as stipulated in IEC60079-14 (proof of intrinsic safety) is mandatory.

### Density compensation with Pt100 temperature sensor

The Waterpilot FMX21 can correct measured errors that result from fluctuations in the density of the water caused by temperature. Users can choose from the following options:


#### Use the internally measured sensor temperature of the FMX21

The internally measured sensor temperature is calculated in the Waterpilot FMX21 for density compensation. The level signal is thus corrected according to the density characteristic line of the water.

#### Use the optional internal temperature sensor for density compensation in a suitable HART master (e.g. PLC)

The Waterpilot FMX21 is available with an optional Pt100 temperature sensor. Endress+Hauser additionally offers the TMT182 temperature head transmitter to convert the Pt100 signal to a 4 to 20 mA HART signal.

The temperature and pressure signals are transmitted to the HART master (e.g. PLC) where a corrected level value can be generated using a stored linearization table or the density function (of a chosen medium).

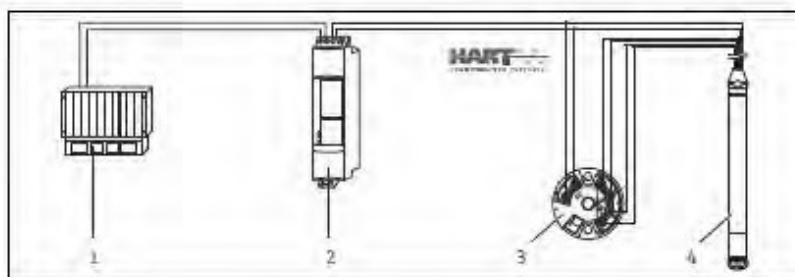


- 1 HART Master, e.g. PLC (programmable logic controller)
- 2 FXN520 Multidrop-Connector
- 3 TMT182 Temperature head transmitter
- 4 Waterpilot FMX21

Use an external temperature signal which is transmitted to the FMX21 via HART burst mode

The Waterpilot FMX21 is available with an optional Pt100 temperature sensor. In this case, the signal of the Pt100 is analyzed using a HART-compliant (at least HART 5.0) temperature transmitter that supports BURST mode. The temperature signal can thus be transmitted to the FMX21. The FMX21 uses this signal for the density correction of the level signal.

 The TMT182 temperature head transmitter is not suitable for this configuration.

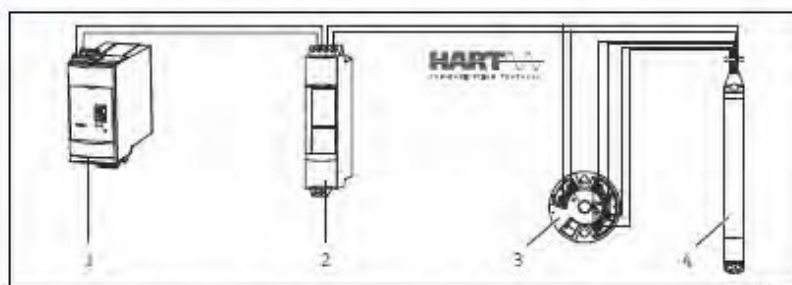

- 1 Fieldgate FXA520
- 2 Multidrop-Connector FXN520
- 3 TMT182 Temperature head transmitter
- 4 Waterpilot FMX21

Without additional compensation due to the anomaly of water, errors of up to 4 % may occur at a temperature of +70 °C (+158 °F), for example. With density compensation, this error can be decreased to 0.5% in the entire temperature range from 0 to +70 °C (+32 to +158 °F).

 For further information please refer to the appropriate Technical documentation:

- TI00078R: TMT182 temperature head transmitter (4 to 20 mA/HART)
- TI00369F: FXA520 Fieldgate
- TI00400F: FXN520 multidrop connector

|                        |                                                                                                              |
|------------------------|--------------------------------------------------------------------------------------------------------------|
| Communication protocol | 4 to 20 mA HART with communication protocol                                                                  |
| System integration     | The device can be fitted with a tag name, 'Ordering information', feature 895 'Marking' version 'Z1' (→ 38). |

## Input

|                   |                                                                                                                |                                                |
|-------------------|----------------------------------------------------------------------------------------------------------------|------------------------------------------------|
| Measured variable | FMX21 + Pt100 (optional)                                                                                       | TMT182 temperature head transmitter (optional) |
|                   | <ul style="list-style-type: none"> <li>Hydrostatic pressure of a liquid</li> <li>Pt100: temperature</li> </ul> | Temperature                                    |

|                 |                                                                                                                                                                                                                                                            |
|-----------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Measuring range | <ul style="list-style-type: none"> <li>Customer-specific measuring ranges or factory calibration</li> <li>Temperature measurement from <math>-10</math> to <math>+70</math> °C (<math>+14</math> to <math>+158</math> °F) with Pt100 (optional)</li> </ul> |
|-----------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|

| Sensor measuring range   | Smallest span that can be calibrated <sup>1)</sup> | Vacuum resistance                          | Version in the order code <sup>2)</sup> |
|--------------------------|----------------------------------------------------|--------------------------------------------|-----------------------------------------|
| [bar (psi)]              | [bar (psi)]                                        | [bar <sub>abs</sub> (psi <sub>abs</sub> )] |                                         |
| <b>Gauge pressure</b>    |                                                    |                                            |                                         |
| 0.1 (1.5)                | 0.01 (0.15)                                        | 0.3 (4.5)                                  | 1C                                      |
| 0.2 (3.0)                | 0.02 (0.3)                                         | 0.3 (4.5)                                  | 1D                                      |
| 0.4 (6.0)                | 0.04 (1.0)                                         | 0                                          | 1F                                      |
| 0.6 (9.0)                | 0.06 (1.0)                                         | 0                                          | 1G                                      |
| 1.0 (15.0)               | 0.1 (1.5)                                          | 0                                          | 1H                                      |
| 2.0 (30.0)               | 0.2 (3.0)                                          | 0                                          | 1K                                      |
| 4.0 (60.0)               | 0.4 (6.0)                                          | 0                                          | 1M                                      |
| 10.0 (150) <sup>3)</sup> | 1.0 (15)                                           | 0                                          | 1P                                      |
| 20.0 (300) <sup>3)</sup> | 2.0 (30)                                           | 0                                          | 1Q                                      |
| <b>Absolute pressure</b> |                                                    |                                            |                                         |
| 2.0 (30.0)               | 0.2 (3.0)                                          | 0                                          | 2K                                      |
| 4.0 (60.0)               | 0.4 (6.0)                                          | 0                                          | 2M                                      |
| 10.0 (150) <sup>3)</sup> | 1.0 (15)                                           | 0                                          | 2P                                      |
| 20.0 (300) <sup>3)</sup> | 2.0 (30)                                           | 0                                          | 2Q                                      |

1) Recommended Turn down: Max 100:1  
Factory calibration Turn down: Max 20:1, higher on request.

2) Ordering information (→ p. 28)

3) These measuring ranges are not offered for the probe version with plastic insulation, outer diameter 29 mm (1.14 in).

|              |                                                                                                              |                                                |
|--------------|--------------------------------------------------------------------------------------------------------------|------------------------------------------------|
| Input signal | FMX21 + Pt100 (optional)                                                                                     | TMT182 temperature head transmitter (optional) |
|              | <ul style="list-style-type: none"> <li>Change in capacitance</li> <li>Pt100: change in resistance</li> </ul> | Pt100 resistance signal, 4-wire                |

## Output

|                 |                                                                                                                                                                                                                                                                             |                                                                                                                                                                                                           |
|-----------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Output signal   | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>4 to 20 mA with overlying digital HART 6.0 communication protocol, 2-wire for hydrostatic pressure measured value</li> <li>Pt100: Temperature-dependent resistance values</li> </ul>                 | <b>TMT182 temperature head transmitter (optional)</b> <p>4 to 20 mA with overlying digital HART 5.0 communication protocol for temperature measured value, 2-wire</p>                                     |
| Signal range    | 3.8 to 20.5 mA                                                                                                                                                                                                                                                              |                                                                                                                                                                                                           |
| Signal on alarm | <b>FMX21 + Pt100 (optional)</b> <p>4 to 20 mA HART<br/>Options:</p> <ul style="list-style-type: none"> <li>Max. alarm (factory setting 22 mA): can be set from 21 to 23 mA</li> <li>Hold measured value: last measured value is held</li> <li>Min. alarm: 3.6 mA</li> </ul> | <b>TMT182 temperature head transmitter (optional)</b> <p>Options:</p> <ul style="list-style-type: none"> <li>Max. alarm <math>\geq 21.0</math> mA</li> <li>Min. alarm <math>\leq 3.6</math> mA</li> </ul> |
| Load            | <b>FMX21</b> $R_{Lmax} \leq \frac{U - 10.5 \text{ V}}{23 \text{ mA}} - 2 \cdot 0.09 \frac{\Omega}{m} \cdot l - R_{add}$ <small>ANEXOS 10</small>                                                                                                                            | <b>TMT182 temperature head transmitter (optional)</b> $R_{Lmax} \leq \frac{U - 11.5 \text{ V}}{0.023 \text{ A}} - R_{add}$ <small>ANEXOS 10</small>                                                       |


$R_{Lmax}$  = Max. load resistance [ $\Omega$ ]

$R_{add}$  = Additional resistances such as resistance of evaluation unit and/or display unit, cable resistance [ $\Omega$ ]


$U$  = Supply voltage [V]

$l$  = Simple length of extension cable [m], (cable resistance per wire  $\leq 0.09 \Omega/m$ )

**i** When using the measuring device in hazardous areas, installation must comply with the corresponding national standards and regulations and the Safety Instructions or Installation or Control Drawings (XA).

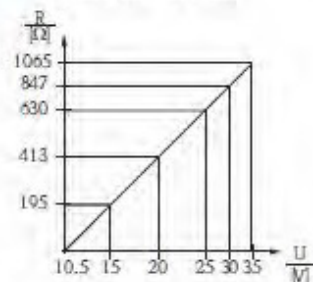

FMX21 load chart for estimating the load resistance. Additional resistances, such as the resistance of the extension cable, have to be subtracted from the value calculated as shown in the equation.

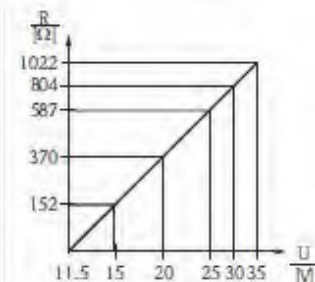

Temperature head transmitter TMT182 load chart for estimating the load resistance. Additional resistances have to be subtracted from the value calculated as shown in the equation.

**i** When operating using a HART handheld terminal or a PC with an operating program, a minimum communication resistance of 250  $\Omega$  has to be taken into account.



|         |                                                                                                                                                                 |
|---------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Damping | <ul style="list-style-type: none"> <li>Continuously 0 to 999 s via HART handheld terminal or PC with operating program</li> <li>Factory setting: 2 s</li> </ul> |
|---------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------|

## Power supply




When using the measuring device in hazardous areas, installation must comply with the applicable national standards and regulations and the Safety Instructions (XAs) and the Installation or Control Drawings (ZDs). All explosion-protection data are given in a separate documentation which is available upon request. This documentation is provided with the devices as standard (→ " 32).

|                                      |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |                                                                                                                                                                                                                                                 |
|--------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Supply voltage                       | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>10.5 to 35 V (non-hazardous area)</li> <li>10.5 to 30 V (hazardous area)</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                      | <b>TMT182 temperature head transmitter (optional)</b><br>11.5 to 35 V DC                                                                                                                                                                        |
| Power consumption                    | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>≤ 0.805 W at 35 V DC (non-hazardous area)</li> <li>≤ 0.690 W at 30 V DC (hazardous area)</li> </ul>                                                                                                                                                                                                                                                                                                                                                                      | <b>TMT182 temperature head transmitter (optional)</b><br>≤ 0.805 W at 35 V DC                                                                                                                                                                   |
| Current consumption                  | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>Max. current consumption: ≤ 23 mA</li> <li>Min. current consumption: ≥ 3.6 mA</li> <li>Pt100: ≤ 0.6 mA</li> </ul>                                                                                                                                                                                                                                                                                                                                                        | <b>TMT182 temperature head transmitter (optional)</b> <ul style="list-style-type: none"> <li>Max. current consumption: ≤ 23 mA</li> <li>Min. current consumption: ≥ 3.5 mA</li> <li>Pt100 via temperature head transmitter: ≤ 0.6 mA</li> </ul> |
| Measuring unit electrical connection | <div> <ul style="list-style-type: none"> <li>Reverse polarity protection is integrated in the Waterpilot FMX21 and in the TMT182 temperature head transmitter. Changing the polarities will not damage the devices.</li> <li>The cable must end in a dry room or a suitable terminal box. The terminal box (IP66/IP67) with a GORE-TEX® filter from Endress+Hauser is suitable for outdoor installations. The terminal box can be ordered as an accessory using the order code for FMX21 version TS for feature 620 (→ " 28).</li> </ul> </div> |                                                                                                                                                                                                                                                 |


The electrical connection is made with the corresponding wires of the probe cable and with the optional use of the terminal box (Commubox FXA) or an active barrier (e.g. RN221N).



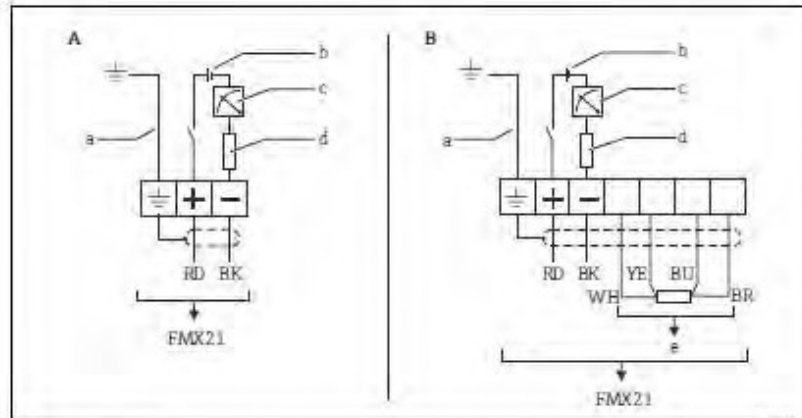

A Waterpilot FMX21  
B Waterpilot FMX21 with Pt100 H-Version<sup>1)</sup> for feature 610 'Accessories' in the order code (→ 128)

- a Not for FMX21 with an outer diameter of 29 mm (1.14 in)  
b 10.5 to 30 V DC (Ex), 10.5 to 35 V DC  
c 4 to 20 mA  
d Resistance ( $R_L$ )  
e Pt100

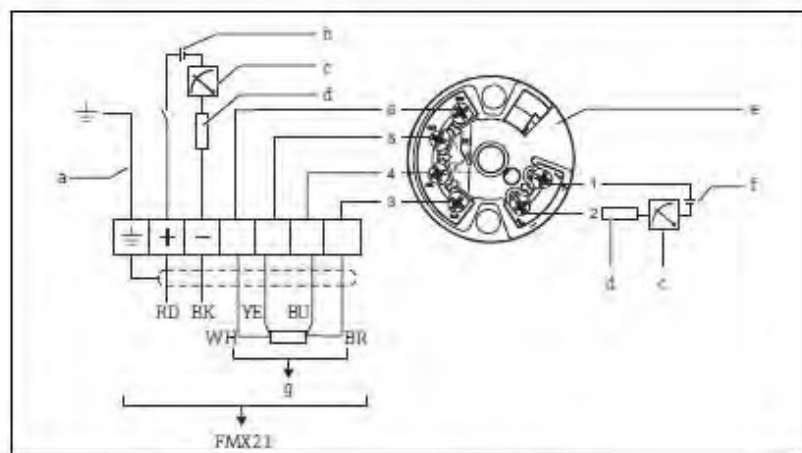

Waterpilot FMX21 with Pt100 and TMT182 temperature head transmitter (4 to 20 mA) <sup>1)</sup>  
versions 'NB' and 'PT', feature 610 and 620 in the order code (→ 128)

- a Not for FMX21 with an outer diameter of 29 mm (1.14 in)  
b 10.5 to 35 V DC  
c 4 to 20 mA  
d Resistance ( $R_L$ )  
e TMT182 temperature head transmitter (4 to 20 mA)  
f 11.5 to 35 V DC  
g Pt100

<sup>1)</sup> Not for use in hazardous areas.

#### Wire colors

RD = red, BK = black, WH = white, YE = yellow, BU = blue, BR = brown

Connection classification as per IEC 61010-1:

- Overvoltage category 1
- Pollution degree 1

## Connection data in the hazardous area

|                |                                                                                                                        |
|----------------|------------------------------------------------------------------------------------------------------------------------|
| 4 to 20 mA     | Ex in EC T4 to T6                                                                                                      |
| U <sub>i</sub> | 30 V DC                                                                                                                |
| I <sub>i</sub> | 133 mA                                                                                                                 |
| P <sub>i</sub> | 1.0 W                                                                                                                  |
| C <sub>i</sub> | 10.3 nF (sensor); 180 pF/m (cable)                                                                                     |
| L <sub>i</sub> | 0 µH (sensor); 1 µH/m (cable)                                                                                          |
| T <sub>a</sub> | -10 °C (+14 °F) ≤ T <sub>a</sub> ≤ +70 °C (+158 °F) for T4; -10 °C (+14 °F) ≤ T <sub>a</sub> ≤ +40 °C (+104 °F) for T6 |

|                      |                                                                                                                                                                                                                                                                                                                |                                                                                                                                                                                                                                         |
|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Cable specifications | FMX21 + Pt100 (optional)                                                                                                                                                                                                                                                                                       | TMT182 temperature head transmitter (optional)                                                                                                                                                                                          |
|                      | <ul style="list-style-type: none"> <li>Commercially available instrument cable</li> <li>Terminal, terminal box: 0.08 to 2.5 mm<sup>2</sup> (28 to 14 AWG)</li> <li>If the Pt100 signal is directly connected to a display and/or evaluation unit, Endress+Hauser recommends using a shielded cable.</li> </ul> | <ul style="list-style-type: none"> <li>Commercially available instrument cable</li> <li>Terminal, terminal box: 0.08 to 2.5 mm<sup>2</sup> (28 to 14 AWG)</li> <li>Transmitter connection: max. 1.75 mm<sup>2</sup> (15 AWG)</li> </ul> |
| Residual ripple      | FMX21 + Pt100 (optional)                                                                                                                                                                                                                                                                                       | TMT182 temperature head transmitter (optional)                                                                                                                                                                                          |
|                      | No impact on the 4 to 20 mA signal to ±5 % residual ripple within the permitted voltage range (according to HART Hardware Specification HCF_SPEC-5+ (DIN IEC 60381-1))                                                                                                                                         | $U_{in} \geq 3 \text{ V}$ at $U \geq 13 \text{ V}$ , $f_{max} = 1 \text{ kHz}$                                                                                                                                                          |


## Performance characteristics

|                                |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |                                                |
|--------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------|
| Reference operating conditions | FMX21 + Pt100 (optional)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              | TMT182 temperature head transmitter (optional) |
|                                | <ul style="list-style-type: none"> <li>As per IEC 60770</li> <li>Ambient temperature T<sub>A</sub> = constant, in range: +21 to +33 °C (+70 °F to +91 °F)</li> <li>Humidity φ = constant, in range: 20 to 80 % RH</li> <li>Ambient pressure p<sub>A</sub> = constant, in range: 860 to 1060 mbar (13 to 16 psi)</li> <li>Position of the measuring cell = constant, in range, vertical: ±1°</li> <li>Supply voltage constant: 21 V DC to 27 V DC</li> <li>Load with HART: 250 Ω</li> <li>Pt100: DIN EN 60770 T<sub>A</sub> = 25 °C (77 °F)</li> </ul> | Calibration temperature 25 °C (77 °F) ±5 K     |

|                                 |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |                                                                                                                                                                                               |
|---------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Reference accuracy              | FMX21 + Pt100 (optional)<br><br>The reference accuracy comprises the non-linearity after limit point configuration, hysteresis and non-repeatability in accordance with IEC 60770.<br><ul style="list-style-type: none"> <li>Setting <math>\pm 0.2\%</math> <ul style="list-style-type: none"> <li>to TD 5:1: <math>&lt; 0.2\%</math> of the set span</li> <li>from TD 5:1 to TD 10:1 <math>\pm(0.02 \times \text{TD} + 0.1)</math></li> </ul> </li> </ul> PLATINUM version:<br><ul style="list-style-type: none"> <li>Setting <math>\pm 0.1\%</math> (optional)               <ul style="list-style-type: none"> <li>to TD 5:1: <math>&lt; 0.1\%</math> of the set span</li> <li>from TD 5:1 to TD 10:1 <math>\pm(0.02 \times \text{TD})</math></li> </ul> </li> <li>Class B to DIN EN 60751               <ul style="list-style-type: none"> <li>Pt100: max. <math>\pm 1\text{ K}</math></li> </ul> </li> </ul> | TMT182 temperature head transmitter (optional)<br><br><ul style="list-style-type: none"> <li><math>\pm 0.2\text{ K}</math></li> <li>With Pt100: max. <math>\pm 0.9\text{ K}</math></li> </ul> |
| Resolution                      | Current output: $1\text{ }\mu\text{A}$<br><br>Read cycle<br>HART commands: 2 to 3 per second on average                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |                                                                                                                                                                                               |
| Long-term stability             | FMX21 + Pt100 (optional)<br><br><ul style="list-style-type: none"> <li><math>\leq 0.1\%</math> of URL/year</li> <li><math>\leq 0.25\%</math> of URL/5 years</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | TMT182 temperature head transmitter (optional)<br><br>$\leq 0.1\text{ K per year}$                                                                                                            |
| Influence of medium temperature | <ul style="list-style-type: none"> <li>Thermal change in the zero output and the output span<br/>               0 to <math>+30\text{ }^{\circ}\text{C}</math> (<math>+32</math> to <math>+86\text{ }^{\circ}\text{F}</math>): <math>&lt;(0.15 + 0.15 \times \text{TD})\%</math><br/>               -10 to <math>+70\text{ }^{\circ}\text{C}</math> (<math>+14</math> to <math>+158\text{ }^{\circ}\text{F}</math>): <math>&lt;(0.4 + 0.4 \times \text{TD})\%</math> </li> <li>Temperature coefficient (<math>T_R</math>) of the zero output and output span<br/>               -10 to <math>+70\text{ }^{\circ}\text{C}</math> (<math>+14</math> to <math>+158\text{ }^{\circ}\text{F}</math>): <math>0.1\%</math> / <math>10\text{ K URL}</math></li> </ul>                                                                                                                                                      |                                                                                                                                                                                               |
| Warm-up period                  | FMX21 + Pt100 (optional)<br><br><ul style="list-style-type: none"> <li>FMX21: <math>&lt; 6\text{ s}</math></li> <li>Pt100: <math>20\text{ ms}</math></li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | TMT182 temperature head transmitter (optional)<br><br>$4\text{ s}$                                                                                                                            |
| Step response time              | FMX21 + Pt100 (optional)<br><br><ul style="list-style-type: none"> <li>FMX21: <math>400\text{ ms}</math> (<math>T_{90}</math> time), <math>500\text{ ms}</math> (<math>T_{99}</math> time)</li> <li>Pt100: <math>160\text{ s}</math> (<math>T_{90}</math> time), <math>300\text{ s}</math> (<math>T_{99}</math> time)</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  | —                                                                                                                                                                                             |

## Installation

### Installation instructions

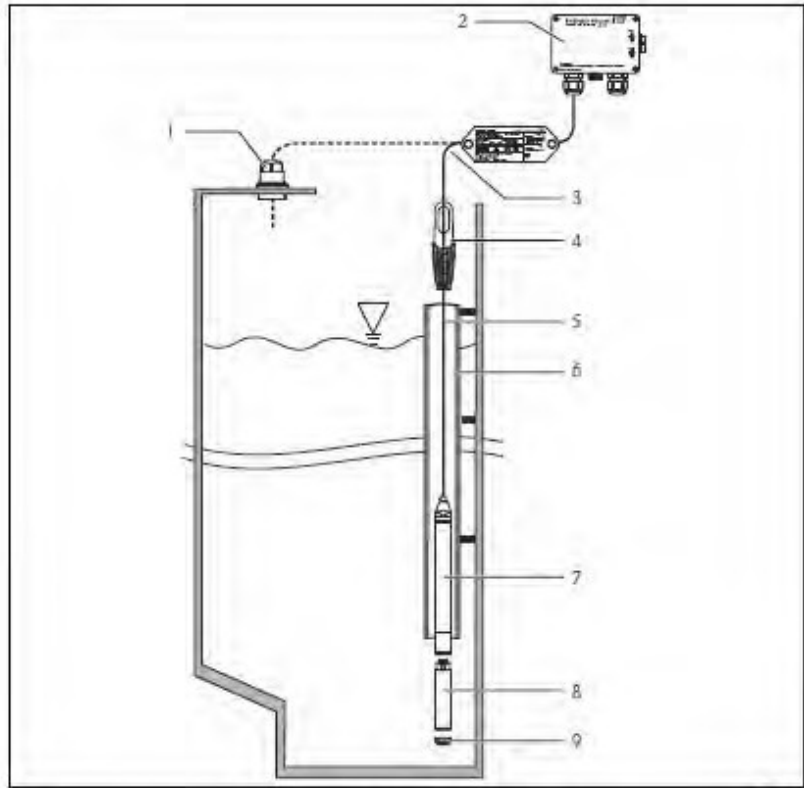

Installation examples, here illustrated with FMX21 with an outer diameter of 22 mm (0.87 in.)

- 1 Extension cable mounting screw can be ordered via order code or as an accessory (→ 28)
- 2 Terminal box can be ordered via order code or as an accessory (→ 28)
- 3 Extension cable bending radius > 120 mm (4.72 in.)
- 4 Mounting clamp can be ordered via order code or as an accessory (→ 28)
- 5 Extension cable, length (→ 25)
- 6 Guide pipe
- 7 Waterpilot FMX21
- 8 Additional weight can be ordered as an accessory for FMX21 with an outer diameter of 22 mm (0.87 in.) and 29 mm (1.14 in.)
- 9 Protection cap

### Additional installation instruction

- Sideways movement of the level probe can result in measuring errors. For this reason, install the probe at a point free from flow and turbulence, or use a guide tube. The internal diameter of the guide tube should be at least 1 mm (0.04 in.) bigger than the outer diameter of the selected FMX21.
- The device is provided with a protection cap to prevent mechanical damage to the measuring cell.
- The cable must end in a dry room or a suitable terminal box. The terminal box from Endress+Hauser provides optimum humidity and climatic protection and is suitable for outdoor installation (→ 30).
- Rod length tolerances: < 5 m (16 ft): ±17.5 mm (0.69 in.); > 5 m (16 ft): ±0.2 % (→ 31)
- If the cable is shortened, the filter at the pressure compensation tube has to be reattached. Endress+Hauser offers a cable shortening kit for this purpose → 28 ff; (SD00552P/00/A6).
- Endress+Hauser recommends using twisted, shielded cables.
- Note for ship building applications: Measures for limitation of the propagation of fire along cable bundles are required (fire stops).

## Environment

|                                                      |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |                                                                                                                                                                                              |
|------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Ambient temperature range</b>                     | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>With outer diameter of 22 mm (0.87 in) and 42 mm (1.65 in):<br/>-10 to +70 °C (+14 to +158 °F)<br/>(= medium temperature)</li> <li>With outer diameter of 29 mm (1.14 in):<br/>0 to +50 °C (+32 to +122 °F)<br/>(= medium temperature)</li> </ul> <b>Cable</b><br>(fixed installation) <ul style="list-style-type: none"> <li>PE: -30 to +70 °C (-22 to +158 °F)</li> <li>FEP: -40 to +70 °C (-40 to +158 °F)</li> <li>PUR: -40 to +70 °C (-40 to +158 °F)</li> </ul> <b>Terminal box</b><br>-40 to +80 °C (-40 to +176 °F) | <b>TMT182 temperature head transmitter (optional)</b><br>-40 to +85 °C (-40 to +185 °F)                                                                                                      |
| <b>Storage temperature range</b>                     | <b>FMX21 + Pt100 (optional)</b><br>-40 to +80 °C (-40 to +176 °F)<br><b>Cable</b><br>(fixed installation) <ul style="list-style-type: none"> <li>PE: -30 to +70 °C (-22 to +158 °F)</li> <li>FEP: -30 to +80 °C (-22 to +176 °F)</li> <li>PUR: -40 to +80 °C (-40 to +176 °F)</li> </ul> <b>Terminal box</b><br>-40 to +80 °C (-40 to +176 °F)                                                                                                                                                                                                                                                     | <b>TMT182 temperature head transmitter (optional)</b><br>-40 to +100 °C (-40 to +212 °F)                                                                                                     |
| <b>Degree of protection</b>                          | <b>FMX21 + Pt100 (optional)</b><br>IP68, permanently hermetically sealed at 20 bar (290 psi) (~200 m H <sub>2</sub> O)<br><b>Terminal box (optional)</b><br>IP66, IP67                                                                                                                                                                                                                                                                                                                                                                                                                             | <b>TMT182 temperature head transmitter (optional)</b><br>IP00, condensation permitted                                                                                                        |
| <b>Geometric height according to IEC61010-1 Ed.3</b> | Up to 2 000 m (6 600 ft) above MSL                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |                                                                                                                                                                                              |
| <b>Electromagnetic compatibility (EMC)</b>           | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>EMC in accordance with all the relevant requirements of the EN 61326 series. Details are provided in the Declaration of Conformity.</li> <li>Maximum deviation &lt; 0.5 % of the span.</li> </ul>                                                                                                                                                                                                                                                                                                                           | <b>TMT182 temperature head transmitter (optional)</b><br>EMC in accordance with all the relevant requirements of the EN 61326 series. Details are provided in the Declaration of Conformity. |



|                        |                                                                                                                                                                                                                                                                     |                                                                                                                     |
|------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------|
| Overvoltage protection | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>Integrated overvoltage protection to EN 61000-4-5 (500 V symmetrical/1000 V asymmetrical)</li> <li>Install overvoltage protection <math>\geq 1.0</math> kV, external if necessary</li> </ul> | <b>TMT182 temperature head transmitter (optional)</b><br><br>Install overvoltage protection, external if necessary. |
|------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------|


## Process

|                          |                                                                                                                                                                                                                                                                    |                                                                |
|--------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------|
| Medium temperature range | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>With outer diameter of 22 mm (0.87 in) and 42 mm (1.65 in):<br/>-10 to +70 °C (+14 to +158 °F)</li> <li>With outer diameter of 29 mm (1.14 in):<br/>0 to +50 °C (+32 to +122 °F)</li> </ul> | <b>TMT182 temperature head transmitter (optional)</b><br><br>— |
|--------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------|

|                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |   |
|---------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---|
| Medium temperature limits | <b>FMX21 + Pt100 (optional)</b> <ul style="list-style-type: none"> <li>With outer diameter of 22 mm (0.87 in) and 42 mm (1.65 in):<br/>-20 to +70 °C (-4 to +158 °F)<br/>  In hazardous areas incl. CSA GP, the medium temperature limit is at -10 to +70 °C (+14 to +158 °F).           </li> <li>With outer diameter of 29 mm (1.14 in):<br/>0 to +50 °C (+32 to +122 °F)<br/>  The FMX21 can be operated in this temperature range. The specification can then be exceeded, e.g. measuring accuracy.           </li> </ul> | — |
|---------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---|

## Mechanical construction

Dimensions of the level probe

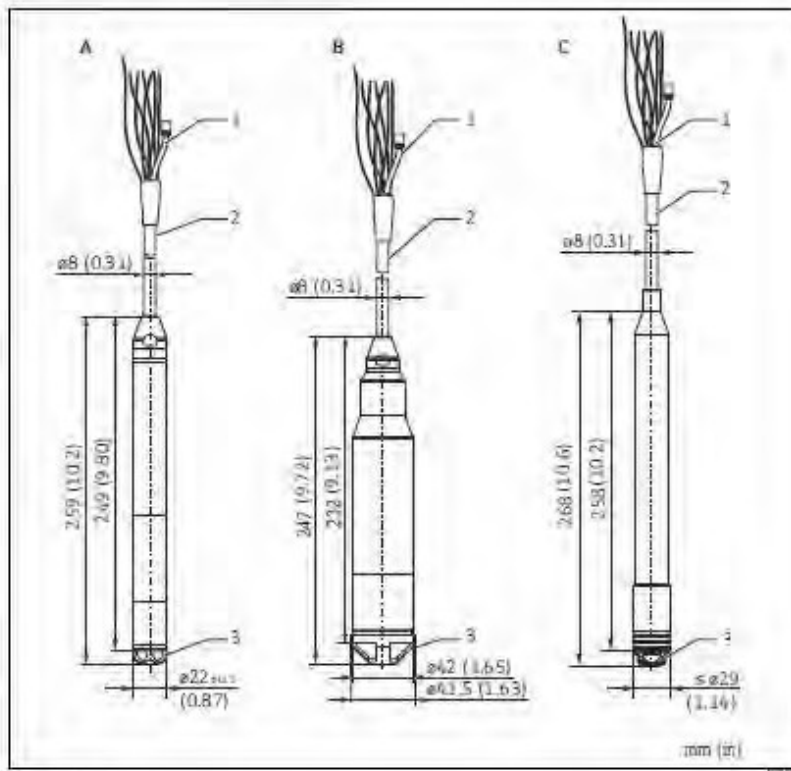


Versions of the FMX11

- A In the order code: feature 45 "Probe tube", version "1" or "Accessories" (→ "28")  
 B In the order code: feature 45 "Probe tube", version "2" (→ "28")  
 C In the order code: feature 45 "Probe tube", version "5" (→ "28")


- 1 Dredging compensation tube  
 2 Extension cable (Length, see → "28")  
 3 Protection cap

Dimensions of the mounting clamp

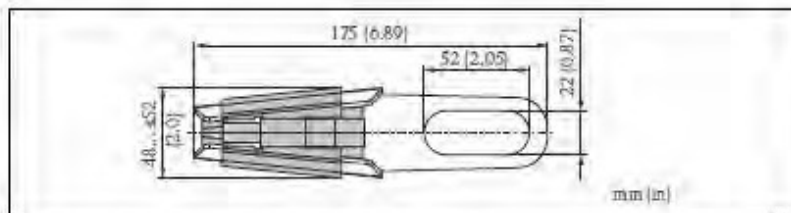

In the order code: feature 620 "Accessories", version "90" (→ "28")


Dimensions of the extension cable mounting screws

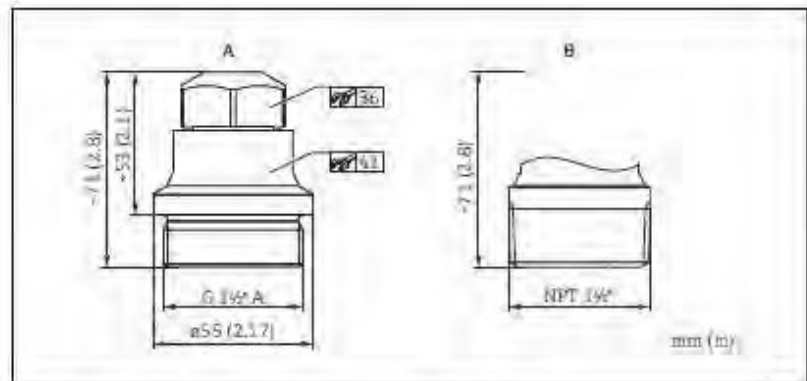

- A G 1/4" A, in the order code: feature 620 'Accessories', version 'P2' (→ '128')  
 B NPT 1/4", in the order code: feature 620 'Accessories', version 'P2' for (→ '128')

**i** Application in unpressurized containers only.

Dimensions of the IP66, IP67 terminal boxes with filters

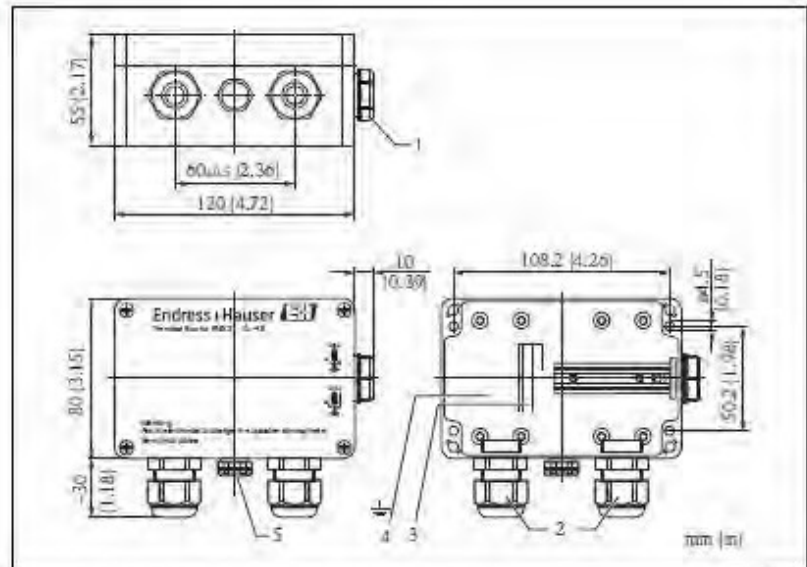


In the order code: feature 620, version 'P2' or 'P1' (→ '128')

- 1 Dummy plug M20x1.5  
 2 Cable gland M20x1.5  
 3 4 to 20 mA; terminals for 0.08 to 2.5 mm<sup>2</sup> (28 to 14 AWG)  
 4 Ground connection; terminals for 0.08 to 2.5 mm<sup>2</sup> (28 to 14 AWG)  
 5 GORE-TEX® filter

If ordered together with FMX21 but without the optional TMT182 temperature transmitter, the terminal box is incl. a 4-terminal strip.


**i** The 4-terminal strip is not intended for use in hazardous areas incl. CSA GP.

Dimensions of the TMT182 temperature head transmitter

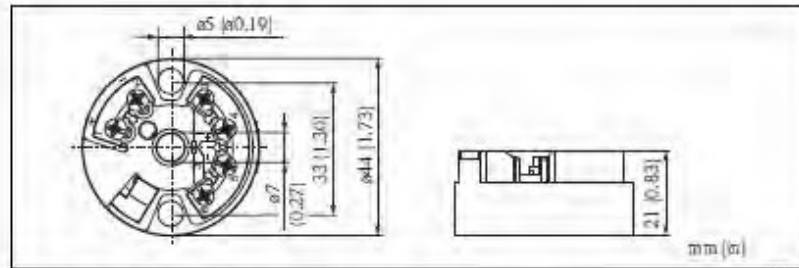

In the order code: feature 020 'Accessories', version: DT for (→ 118)

Terminal box with integrated TMT182 temperature head transmitter (4 to 20 mA HART)

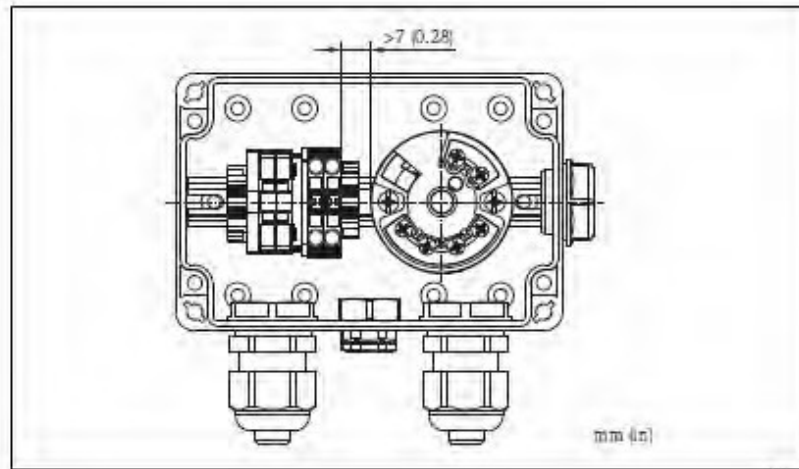


 A distance of > 7 mm (> 0.28 in mm) must be maintained between the terminal strip and the TMT182 temperature head transmitter.

Weight

| Component part                              | Weight                                                                               |
|---------------------------------------------|--------------------------------------------------------------------------------------|
| Level probe, outer diameter 22 mm (0.87 in) | 344 g (12.133 oz)                                                                    |
| Level probe, outer diameter 42 mm (1.65 in) | 1376 g (48.532 oz)                                                                   |
| Level probe, outer diameter 29 mm (1.14 in) | 394 g (13.896 oz)                                                                    |
| Extension cable                             | <ul style="list-style-type: none"> <li>■ PE</li> <li>■ PUR</li> <li>■ FEP</li> </ul> |
| Mounting clamp                              | 170 g (5.996 oz)                                                                     |
| Extension cable mounting screw G 1/4" A     | 770 g (27.158 oz)                                                                    |
| Extension cable mounting screw NPT 1/4"     | 724 g (25.535 oz)                                                                    |
| Terminal box                                | 235 g (8.288 oz)                                                                     |
| Temperature head transmitter TMT182         | 40 g (1.411 oz)                                                                      |
| Additional weight                           | 300 g (10.581 oz)                                                                    |
| Testing adapter                             | 39 g (1.376 oz)                                                                      |


Material

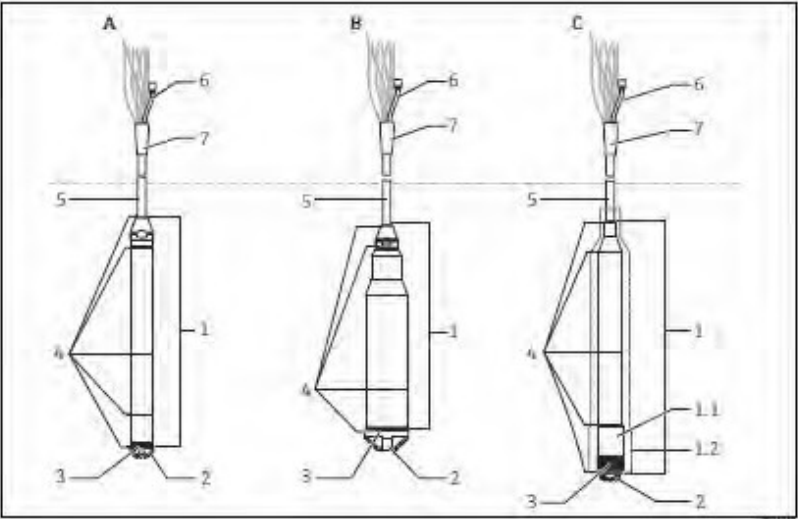

| Material in contact with process     |                                                                                                                                                                                                                                                                |                                                                                                                                                                  |
|--------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Position number                      | Component part                                                                                                                                                                                                                                                 | Material                                                                                                                                                         |
| 1                                    | A: Level probe, outer diameter 22 mm (0.87 in)<br>B: Level probe, outer diameter 42 mm (1.65 in)<br>C: Level probe, outer diameter max. 29 mm (1.14 in)                                                                                                        | 316L (1.4404/1.4435)                                                                                                                                             |
| 1.1                                  | Sensor sleeve                                                                                                                                                                                                                                                  | PFS (polyphenylene sulfide)                                                                                                                                      |
| 1.2                                  | Heat-shrink sleeve                                                                                                                                                                                                                                             | Polyolefin and hot-melt adhesive                                                                                                                                 |
|                                      |  The heat-shrink sleeve at the level probe acts as an insulation. It prevents electrical contact between the probe and the tank. Electrochemical corrosion is thus avoided. |                                                                                                                                                                  |
| 2                                    | Protection cap <ul style="list-style-type: none"><li>A and C: with outer diameter 22 mm (0.87 in) and 29 mm (1.14 in)</li><li>B: with outer diameter 42 mm (1.65 in)</li></ul>                                                                                 | <ul style="list-style-type: none"><li>PPO (Polyphenylenoxid)</li><li>FFA (Perfluoralkoxy)</li></ul>                                                              |
| 3                                    | Process ceramic                                                                                                                                                                                                                                                | Al <sub>2</sub> O <sub>3</sub> (aluminum oxide ceramic)                                                                                                          |
| 4                                    | Seal                                                                                                                                                                                                                                                           | EPDM or FKM Viton                                                                                                                                                |
| 5                                    | Extension cable insulation<br><br>For more information → <a href="#">p. 25</a>                                                                                                                                                                                 | Either: <ul style="list-style-type: none"><li>PE-LD (low-density polyethylene)</li><li>FEP (fluorinated ethylene propylene)</li><li>PUR (polyurethane)</li></ul> |
| Material not in contact with process |                                                                                                                                                                                                                                                                |                                                                                                                                                                  |
| 6                                    | Pressure compensation tube                                                                                                                                                                                                                                     | PA                                                                                                                                                               |
| 7                                    | Heat-shrink sleeve                                                                                                                                                                                                                                             | Polyolefin                                                                                                                                                       |




Terminal box (not in contact with process)

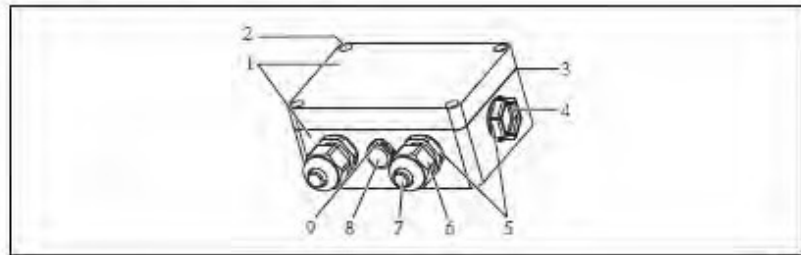

401389.02

| Position number | Component part                    | Material                            |
|-----------------|-----------------------------------|-------------------------------------|
| 1               | Housing                           | PC                                  |
| 2               | Mounting screws (4 x)             | A2                                  |
| 3               | Seal                              | CR (Chloropren-Unvulcanized rubber) |
| 4               | Dummy plug M20x1.5                | PBT-GF30                            |
| 5               |                                   | PE-HD                               |
| 6               | Cable gland M20x1.5               | PA6                                 |
| 7               |                                   | PA6-GF30                            |
| 8               | Pressure compensation tube        | PA6-GF10, ePTFE                     |
| 9               | Pressure compensation tube O-ring | Silicone (VMQ)                      |

Cable mounting screw (not in contact with process)

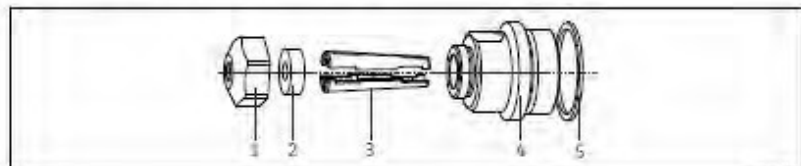


401389.02

| Position number | Component part                                       | Material     |
|-----------------|------------------------------------------------------|--------------|
| 1               | Cover cable gland                                    | 304 (1.4301) |
| 2               | Seal                                                 | NBR          |
| 3               | Klemmhülse                                           | PA66-GF35    |
| 4               | Anschlussstück cable gland<br>G 1 1/4" A, NPT 1 1/2" | 304 (1.4301) |
| 5               | Seal → only for G 1 1/4" A                           | EPDM         |

## Extension cable

| PE                                                                                                                                                                                                                                                                                                                  | PUR                                                                                                                                                                                                                                                                                                                  | FEP                                                                                                                                                                                                                                                                                                           |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <ul style="list-style-type: none"> <li>• Abrasion-resistant extension cable with Dynema strain-relief members</li> <li>• Shielded with aluminum-coated film</li> <li>• Insulated with polyethylene (PE), black</li> <li>• Copper wires, twisted</li> <li>• Pressure compensation tube with Teflon filter</li> </ul> | <ul style="list-style-type: none"> <li>• Abrasion-resistant extension cable with Dynema strain-relief members</li> <li>• Shielded with aluminum-coated film</li> <li>• Insulated with polyurethane (PUR), black</li> <li>• Copper wires, twisted</li> <li>• Pressure compensation tube with Teflon filter</li> </ul> | <ul style="list-style-type: none"> <li>• Abrasion-resistant extension cable</li> <li>• Shielded with galvanized steel wire netting</li> <li>• Insulated with fluorinated ethylene propylene (FEP), black</li> <li>• Copper wires, twisted</li> <li>• Pressure compensation tube with Teflon filter</li> </ul> |

## Cable length

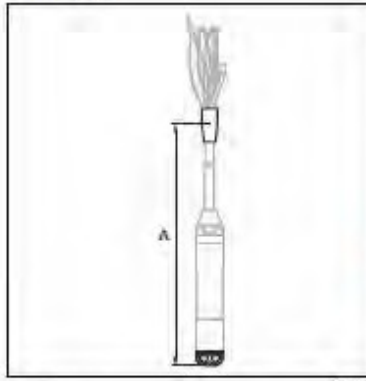

A Cable length

- Please refer also to 'Load' (→ 12).
- Cable lengths that can be ordered
  - Customer-specific length in meters or feet (→ 26, 'Ordering information')
  - Limited cable length when performing installation with freely suspended device with extension cable mounting screw or mounting clamp, as well as for hazardous areas: max. 300 m (984 ft).

**i** When using the measuring device in hazardous areas, installation must comply with the applicable national standards and regulations and the Safety Instructions (XAs) or the Installation or Control Drawings (ZDs) 'Documentation'

## Cross-section

- Total outer diameter: 8.0 mm (0.31 in)  $\pm 0.25$  mm ( $\pm 0.01$  in)
- FMX21: 3 x 0.227 mm<sup>2</sup> (3 x 26 AWG) + pressure compensation tube with Teflon filter
- FMX21 with Pt100 (optional): 7 x 0.227 mm<sup>2</sup> (7 x 26 AWG) + pressure compensation tube with Teflon filter
- Pressure compensation tube with Teflon filter:
  - outer diameter 2.5 mm (0.1 in), internal diameter 1.5 mm (0.06 in)

## Cable resistance

per wire:  $\leq 0.09 \Omega/\text{m}$

## Further technical data

- Minimum bending radius: 120 mm (4.72 in)
- Tensile strength: max. 950 N (213.56 lbf)
- Cable extraction force (= necessary tensile force to extract the cable from the level probe):
  - PE, FEP: typical  $\geq 400$  N (89.92 lbf), PUR: typical  $\geq 150$  N (33.72 lbf)
  - for use in hazardous areas:  $\geq 100$  N (22.48 lbf)
- Resistance to UV light
- PE: Usage in drinking water

## Terminals

- Three terminals as standard in the terminal box
- 4-terminal strip can be ordered as an accessory, Order No: 52008938  
Conductor cross-section 0.08 to 2.5 mm<sup>2</sup> (28 to 14 AWG)



The 4-terminal strip is not intended for use in hazardous areas incl. CSA GP.

---

## Operability

---

|                        |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
|------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>FieldCare</b>       | <p>FieldCare is Endress+Hauser's plant asset management tool based on FDT technology. You can use FieldCare to configure all Endress+Hauser devices as well as third-party devices which support the FDT standard.</p> <p>FieldCare supports the following functions:</p> <ul style="list-style-type: none"><li>■ Configuration of transmitters in offline and online mode</li><li>■ Loading and saving device data (upload/download)</li><li>■ Documentation of the measuring point</li></ul> <p>Connection options:</p> <ul style="list-style-type: none"><li>■ Via Commubox FXA195 and the USB port of a computer</li><li>■ Via Fieldgate FXA520</li></ul> <p>For further information and free download of FieldCare see → <a href="http://www.endress.com">www.endress.com</a> → Download → Search: FieldCare</p> |
| <b>Field Xpert SFX</b> | <p>Field Xpert is an industrial PDA with integrated 3.5" touchscreen from Endress+Hauser based on Windows Mobile. It communicates via wireless with the optional VIATOR® Bluetooth® modem, connected to a HART device point-to-point or wireless via WiFi and Endress+Hauser's Fieldgate FXA520. Field Xpert also works as a stand-alone device for asset management applications. For details refer to BA000605/00/EN.</p>                                                                                                                                                                                                                                                                                                                                                                                           |

## Certificates and approvals

|                                 |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
|---------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>CE mark</b>                  | The device meets the legal requirements of the applicable EC Directives. Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
| <b>Ex approval</b>              | <ul style="list-style-type: none"> <li>■ ATEX</li> <li>■ CSA C/US</li> <li>■ FM</li> <li>■ IEC</li> <li>■ NEPSI</li> <li>■ INMETRO</li> </ul> <p> The approvals to apply only for Waterpilot FMX21 without Pt100 and without IMT182.</p> <ul style="list-style-type: none"> <li>■ Waterpilot FMX21 is only available for use in hazardous areas with the FKM Viton seal.</li> <li>■ All explosion protection data are given in separate documentation which is available upon request. The Ex documentation is supplied as standard with all devices approved for use in explosion hazardous areas (→ <a href="#">p. 32</a>).</li> </ul>                                                                                                                                                                                                        |
| <b>Drinking water approval</b>  | <p>For FMX21 with outer diameter 22 mm (0.87 in)</p> <ul style="list-style-type: none"> <li>■ KTW certificate</li> <li>■ NSF 61 approval</li> <li>■ ACS approval</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>Marine certificate</b>       | <ul style="list-style-type: none"> <li>■ GL (Germanischer Lloyd)</li> <li>■ ABS (American Bureau of Shipping)</li> <li>■ LR (Lloyds Register)</li> <li>■ BV (Bureau Veritas)</li> <li>■ DNV (Det Norske Veritas)</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>Standards and guidelines</b> | <p>The European standards and guidelines that have been applied are listed in the associated EC Declarations of Conformity. In addition, the following standards were also applied for the Waterpilot FMX21:</p> <ul style="list-style-type: none"> <li>■ DIN EN 60770 (IEC 60770):<br/>Transmitters for use in industrial process control systems<br/>Part 1: Methods for performance evaluation</li> <li>■ DIN 16086:<br/>Electrical pressure measuring instruments,<br/>pressure sensors, pressure transmitters,<br/>pressure measuring instruments, concepts, specifications on data sheets</li> <li>■ EN 61326:<br/>Electrical equipment for measurement, control and laboratory use – EMC requirements</li> <li>■ EN 61010-1 (IEC 61010-1):<br/>Safety requirements for electrical equipment for measurement, control and laboratory use</li> <li>■ IEC 60529:<br/>Degrees of protection provided by enclosures</li> </ul> |

## Ordering information

FMX21

You can enter the versions for the specific feature in the following table. The versions entered make up the complete order code. Options which are mutually exclusive are not marked.

|        |                            |                                                                                                        |  |            |
|--------|----------------------------|--------------------------------------------------------------------------------------------------------|--|------------|
| 10     | <b>Approval:</b>           |                                                                                                        |  |            |
|        | AA                         | Non-hazardous area                                                                                     |  |            |
|        | BE                         | ATEX II 2 G Ex ia IIC TB                                                                               |  |            |
|        | BD                         | ATEX II 3 G Ex ia IIC TB                                                                               |  |            |
|        | FE                         | FM 1S, CL I Division 1, Groups A - D; AEX II, zone 1                                                   |  |            |
|        | CE                         | CSA C/US 35-CI, I Division 1, Groups A - D, Ex ia, zone 1                                              |  |            |
|        | CD                         | CSA - General Purpose                                                                                  |  |            |
|        | IC                         | IEC Ex ia IIE T5 Gb                                                                                    |  |            |
|        | MA                         | INMETEC Ex ia IIC TB                                                                                   |  |            |
|        | NA                         | NEPSI Ex ia IIC TB                                                                                     |  |            |
| 20     | <b>Output:</b>             |                                                                                                        |  |            |
|        | 2                          | 4-20 mA HART                                                                                           |  |            |
| 45     | <b>Probe tube:</b>         |                                                                                                        |  |            |
|        | 1                          | Outer diameter $\varnothing = 22$ mm, AISI 316L                                                        |  |            |
|        | 2                          | Outer diameter $\varnothing = 42$ mm, flush-mounted, AISI 316L                                         |  |            |
|        | 3                          | Outer diameter $\varnothing = 29$ mm, AISI 316L, FFS/polyolefin for saltwater applications             |  |            |
| 70     | <b>Sensor range:</b>       |                                                                                                        |  |            |
|        | <b>Measuring range</b>     |                                                                                                        |  |            |
|        | 1C                         | 100 mbar/10 kPa/1.5 psi gauge, 1 m H <sub>2</sub> O/3 ft H <sub>2</sub> O/40 in H <sub>2</sub> O       |  |            |
|        | 1D                         | 200 mbar/20 kPa/3 psi gauge, 2 m H <sub>2</sub> O/6 ft H <sub>2</sub> O/80 in H <sub>2</sub> O         |  |            |
|        | 1F                         | 400 mbar/40 kPa/6 psi gauge, 4 m H <sub>2</sub> O/13 ft H <sub>2</sub> O/160 in H <sub>2</sub> O       |  |            |
|        | 1C                         | 500 mbar/50 kPa/9 psi gauge, 5 m H <sub>2</sub> O/17 ft H <sub>2</sub> O/240 in H <sub>2</sub> O       |  |            |
|        | 1H                         | 1 bar/100 kPa/15 psi gauge, 10 m H <sub>2</sub> O/33 ft H <sub>2</sub> O/400 in H <sub>2</sub> O       |  |            |
|        | 1K                         | 2 bar/200 kPa/30 psi gauge, 20 m H <sub>2</sub> O/67 ft H <sub>2</sub> O/800 in H <sub>2</sub> O       |  |            |
|        | 1M                         | 4 bar/400 kPa/60 psi gauge, 40 m H <sub>2</sub> O/133 ft H <sub>2</sub> O/1600 in H <sub>2</sub> O     |  |            |
|        | 1P                         | 10 bar/1 MPa/150 psi gauge, 100 m H <sub>2</sub> O/333 ft H <sub>2</sub> O/4000 in H <sub>2</sub> O    |  |            |
|        | 1Q                         | 20 bar/2 MPa/300 psi gauge, 200 m H <sub>2</sub> O/667 ft H <sub>2</sub> O/8000 in H <sub>2</sub> O    |  |            |
|        | 2K                         | 2 bar/200 kPa/30 psi absolute, 20 m H <sub>2</sub> O/67 ft H <sub>2</sub> O/800 in H <sub>2</sub> O    |  |            |
|        | 2M                         | 4 bar/400 kPa/60 psi absolute, 40 m H <sub>2</sub> O/133 ft H <sub>2</sub> O/1600 in H <sub>2</sub> O  |  |            |
|        | 2P                         | 10 bar/1 MPa/150 psi absolute, 100 m H <sub>2</sub> O/333 ft H <sub>2</sub> O/4000 in H <sub>2</sub> O |  |            |
|        | 2Q                         | 20 bar/2 MPa/300 psi absolute, 200 m H <sub>2</sub> O/667 ft H <sub>2</sub> O/8000 in H <sub>2</sub> O |  |            |
| 80     | <b>Reference accuracy:</b> |                                                                                                        |  |            |
|        | D                          | Platinum                                                                                               |  |            |
|        | G                          | Standard                                                                                               |  |            |
| 90     | <b>Calibration, unit:</b>  |                                                                                                        |  |            |
|        | A                          | Sensor range: %                                                                                        |  |            |
|        | B                          | Sensor range: mbar/bar                                                                                 |  |            |
|        | C                          | Sensor range: kPa/MPa                                                                                  |  |            |
|        | D                          | Sensor range: mm/mH <sub>2</sub> O                                                                     |  |            |
|        | E                          | Sensor range: in H <sub>2</sub> O/ft H <sub>2</sub> O                                                  |  |            |
|        | F                          | Sensor range: psi                                                                                      |  |            |
|        | J                          | Customized pressure; see additional specification                                                      |  |            |
|        | K                          | Customized level; see additional specification                                                         |  |            |
| FMX21- |                            |                                                                                                        |  | Order code |

→ Ordering information for continued on next page



---

---

## Accessories

### Mounting clamp


- Endress+Hauser offers a mounting clamp for easy FMX21 mounting (→ 20).
- Material: 316L (1.4404) and fiberglass reinforced PA (polyamide)
- Order number 52006151, 'Ordering information' (→ 28)

### Terminal box

- IP66/IP67 terminal boxes with GORE-TEX® filter incl. 3 integrated terminals. The terminal box is also suitable for installing a TMT182 temperature head transmitter or for four additional terminals (Order No. 52008938) → 21, 'Ordering information' (→ 28).

**i** The terminal box is not intended for the FMX21 with Ex nA explosion protection in the hazardous area. When using the terminal box in hazardous areas, installation must comply with the corresponding national standards and regulations and the Safety Instructions or Installation or Control Drawings.

### Additional weight

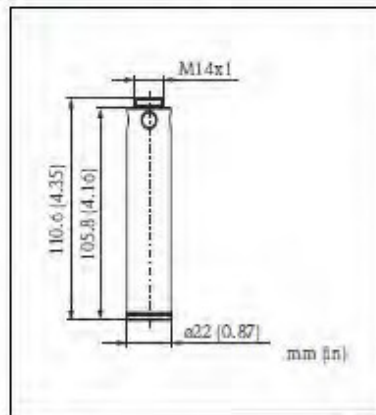

For FMX21 with outer diameter of 22 mm (0.87 in) or 29 mm (1.14 in)

- Endress+Hauser offers additional weights to prevent sideways movement that results in measuring errors, or to make it easier to lower the device in a guide tube. You can screw several weights together. The weights are attached directly to the FMX21. For FMX21 with an outer diameter of 29 mm (1.14 in) a maximum of 5 weights may be attached. In combination with the Ex nA approval, for FMX21 with an outer diameter of 29 mm (1.14 in) a maximum of 1 additional weight may be attached.
- Material: 316L (1.4435)
- Weight: 300 g (10.581 oz)
- Order number 52006153, 'Ordering information' (→ 28)

### TMT182 temperature head transmitter (4 to 20 mA HART)

- 2-wire temperature head transmitter, configured for a measuring range from -20 to +80 °C (-4 to +158 °F). This setting offers a temperature range of 100 K which can be easily mapped. Please note that the Pt100 resistance thermometer is designed for a temperature range from -10 to +70 °C (-14 to +176 °F) → 22.
- Order number: 51001023, 'Ordering information' (→ 28)

**i** The TMT182 temperature head transmitter is not intended for use in hazardous areas incl. CSA GP.

### Extension cable mounting screw

- Endress+Hauser offers extension cable mounting screws to ease FMX21 mounting and to seal the measuring aperture (→ 21).
- Order number for extension cable mounting screw:
    - 52008264 (G 1½" A)
    - 52009311 (NPT 1½")
  - Material (→ 23)

### Terminals

- Four terminals in strip for terminal box, suitable for wire cross-section: 0.08 to 2.5 mm<sup>2</sup> (28 to 14 AWG)
- Order number: 52008938


**i** The 4-terminal strip is not intended for use in hazardous areas incl. CSA GP.

#### Cable shortening kit

- The cable shortening kit is used to easily and professionally shorten a cable.
- Order Number: 71222671, "Ordering information" and the documentation SD00552F/00/A6 (→ 28)

 The cable shortening kit is not intended for the FMX21 with FM/CSA approval.

#### Cable marking

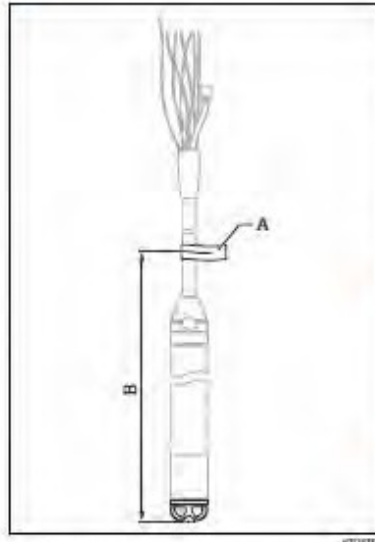

A Cable marking  
B Cable marking tolerance

- To make installation easier, Endress+Hauser offers a mark on the extension cable for a customer-specific length, see also → 28, "Ordering information".
- Cable marking tolerance (distance to the lower end of the cable probe):  
Cable length < 5 m (16 ft):  $\pm 17.5$  mm (0.69 in)  
Cable length > 5 m (16 ft):  $\pm 0.2$  %
- Material: PET, Adhesive: acrylic
- Immunity to temperature change:  
-30 to +100 °C (-22 to +212 °F)


#### NOTICE

The mark is for installation purposes only.

- It must be thoroughly removed without trace in the case of devices with drinking water approval. The extension cable must not be damaged in the process

 Not for use in hazardous areas.

#### Testing adapter

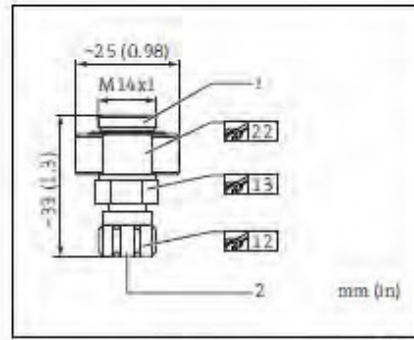

1 FMX21 level probe connection  
2 Compressed air hose connection, internal diameter of quick coupling piece 4 mm (0.16 in)

For FMX21 with outer diameter of 22 mm (0.87 in) and 29 mm (1.14 in)

- Endress+Hauser offers a testing adapter to ease function-testing of the level probes.
- Observe the maximum pressure for the compressed air hose and the maximum overload for the level probe (→ 11).
- Maximum pressure of the quick coupling piece supplied: 10 bar (145 psi)
- Adapter material: 304 (1.4301)
- Quick coupling piece material: anodized aluminum
- Adapter weight: 39 g (1.376 oz)
- Order number 52011868 (→ 28)

## Documentation

The following document types are also available in the Download Area of the Endress+Hauser website: [www.endress.com](http://www.endress.com) → Download

|                        |                                                                                                                                                                                                                                 |
|------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Field of activities    | <ul style="list-style-type: none"> <li>Pressure measurement: FA00004P/00/EN</li> <li>Recording technology: FA00014R/09/EN</li> <li>System components: FA00016K/09/EN</li> </ul>                                                 |
| Technical Information  | <ul style="list-style-type: none"> <li>Waterpilot FMX167 with 4 to 20 mA analog output: TI00351P/00/EN</li> <li>Deltapilot M: TI00437P/00/EN</li> <li>Temperature head transmitter ITEMP HART TMT182: TI00078R/09/EN</li> </ul> |
| Operating Instructions | <ul style="list-style-type: none"> <li>Waterpilot FMX21: BA00380P/00/EN</li> <li>Cable shortening kit: SD00552P/00/A6</li> <li>Field Xpert: BA012115/04/EN</li> </ul>                                                           |
| Safety instructions    | Safety Instructions (XA) are supplied with the device depending on the approval. These instructions are an integral part of the Operating Instructions.                                                                         |

| Approval | Feature in Order code | Type of protection | Category | Documentation      |
|----------|-----------------------|--------------------|----------|--------------------|
| ATEX     | BD                    | Ex ia IIC          | II 2 G   | XA00454P           |
| ATEX     | BE                    | Ex nA IIC          | II 3 G   | XA00485P           |
| IECEX    | IC                    | Ex ia IIC          | n/a      | XA00455P           |
| CSA C/US | CE                    | Ex ia IIC          | n/a      | ZD231P (960008976) |
| FM       | FE                    | AEx ia IIC         | n/a      | ZD231P (960008975) |
| NEPSI    | MA                    | Ex ia IIC          | n/a      | XA00456P           |
| DNVMEIRO | MA                    | Ex ia IIC          | n/a      | XA01066P           |



The nameplate provides information on the Safety Instructions (XA) that are relevant for the device.

|                         |                                                                                                                                     |
|-------------------------|-------------------------------------------------------------------------------------------------------------------------------------|
| Drinking water approval | <ul style="list-style-type: none"> <li>SD00289P/00/A3 (NSF)</li> <li>SD00319P/00/A3 (KITW)</li> <li>SD00320P/00/A3 (ACS)</li> </ul> |
|-------------------------|-------------------------------------------------------------------------------------------------------------------------------------|

## Patents

This product is protected by at least one of the following patents. Further patents are pending.

- US 6,427,129 B1 & EP 0 892 249 B1
- US 6,703,943 A1
- DE 203 13 744.2 U1

## Configuration data sheet

### Level

The following configuration data sheet has to be filled in and included with the order if the option 'K: customized level' has been selected in feature '090: Calibration; unit' in the product structure.

| Pressure Engineering Unit                                                     |                                             |                                              |                              | Output Unit (Scaled unit)                                                |                               |                                          |                               |                            |
|-------------------------------------------------------------------------------|---------------------------------------------|----------------------------------------------|------------------------------|--------------------------------------------------------------------------|-------------------------------|------------------------------------------|-------------------------------|----------------------------|
| <input type="checkbox"/> mbar                                                 | <input type="checkbox"/> mmH <sub>2</sub> O | <input type="checkbox"/> mmHg                | <input type="checkbox"/> hPa | Mass                                                                     | Length                        | Volume                                   | Volume                        | Percent                    |
| <input type="checkbox"/> bar                                                  | <input type="checkbox"/> mH <sub>2</sub> O  |                                              | <input type="checkbox"/> kPa | <input type="checkbox"/> kg                                              | <input type="checkbox"/> m    | <input type="checkbox"/> l               | <input type="checkbox"/> gal  | <input type="checkbox"/> % |
|                                                                               | <input type="checkbox"/> ftH <sub>2</sub> O |                                              | <input type="checkbox"/> MPa | <input type="checkbox"/> t                                               | <input type="checkbox"/> dm   | <input type="checkbox"/> hl              | <input type="checkbox"/> lgal |                            |
| <input type="checkbox"/> psi                                                  | <input type="checkbox"/> inH <sub>2</sub> O | <input type="checkbox"/> kgf/cm <sup>2</sup> |                              | <input type="checkbox"/> lb                                              | <input type="checkbox"/> cm   |                                          |                               |                            |
|                                                                               |                                             |                                              |                              |                                                                          | <input type="checkbox"/> mm   | <input type="checkbox"/> m <sup>3</sup>  |                               |                            |
|                                                                               |                                             |                                              |                              |                                                                          |                               | <input type="checkbox"/> ft <sup>3</sup> |                               |                            |
|                                                                               |                                             |                                              |                              |                                                                          | <input type="checkbox"/> ft   | <input type="checkbox"/> in <sup>3</sup> |                               |                            |
|                                                                               |                                             |                                              |                              |                                                                          | <input type="checkbox"/> inch |                                          |                               |                            |
| Empty calibration (a):<br>low pressure value (empty) _____<br>[pres.eng.unit] |                                             |                                              |                              | Empty calibration (a):<br>low level value (empty) _____<br>[scaled unit] |                               |                                          |                               |                            |
| Full calibration (b):<br>high pressure value (full) _____<br>[pres.eng.unit]  |                                             |                                              |                              | Full calibration (b):<br>high level value (full) _____<br>[scaled unit]  |                               |                                          |                               |                            |
| <b>Damping</b>                                                                |                                             |                                              |                              |                                                                          |                               |                                          |                               |                            |
| Damping: _____ sec                                                            |                                             |                                              |                              |                                                                          |                               |                                          |                               |                            |

### Pressure

The following configuration data sheet has to be filled in and included with the order if the option 'J: customized pressure' has been selected in feature '090: Calibration; unit' in the product structure.

| Pressure Engineering Unit         |                                             |                                              |                              |
|-----------------------------------|---------------------------------------------|----------------------------------------------|------------------------------|
| <input type="checkbox"/> mbar     | <input type="checkbox"/> mmH <sub>2</sub> O | <input type="checkbox"/> mmHg                | <input type="checkbox"/> Pa  |
| <input type="checkbox"/> bar      | <input type="checkbox"/> mH <sub>2</sub> O  |                                              | <input type="checkbox"/> kPa |
|                                   | <input type="checkbox"/> ftH <sub>2</sub> O |                                              | <input type="checkbox"/> MPa |
| <input type="checkbox"/> psi      | <input type="checkbox"/> inH <sub>2</sub> O | <input type="checkbox"/> kgf/cm <sup>2</sup> |                              |
| <b>Calibration Range / Output</b> |                                             |                                              |                              |
| Low range value (LRV) _____       |                                             | [pressure engineering unit]                  |                              |
| Upper range value (URV) : _____   |                                             | [pressure engineering unit]                  |                              |
| <b>Damping</b>                    |                                             |                                              |                              |
| Damping: _____ sec                |                                             |                                              |                              |



## Final Inspection Report / Endprüfprotokoll

The manufacturer confirms that all measuring equipment used to assure the quality of the products has been calibrated and is traceable to national (e.g. DKD/DALIS, NIST, NABL...) or international standards.

Der Hersteller bestätigt, dass die zu Qualitätsprüfungen des Erzeugnisses eingesetzten Messmittel gültig kalibriert waren und auf nationale (z.B. DKD/DALIS, NIST, NABL...) bzw. internationale Normale rückführbar sind.

### Waterpilot HART

|                           |                               |                            |
|---------------------------|-------------------------------|----------------------------|
| TAG number                | Messstellen-Nummer            |                            |
| Order code                | Bestellcode                   | FMX21-6FF0/0               |
| Serial number             | Seriennummer                  | NB00D915122                |
| Extended order code       | Erweiterter Bestellcode       | FMX21-FE211HGE25A+PO       |
| Sensor range              | Sensor-Messbereich            | 0...400 inH <sub>2</sub> O |
| Adjusted measuring range  | Eingestellter Messbereich     | 0...400 inH <sub>2</sub> O |
| Maximum permissible error | Max. zulässige Messabweichung | ± 0.2 %                    |
| Output type               | Ausgang                       | 4-20 mA HART               |
| Software version          | Softwareversion               | 01.00                      |
| Output mode               | Ausgangsmodus                 | linear                     |

### HAMPTON ROADS SANITATION DISTRICT HRSD

|                                                                                                     |                           |                           |
|-----------------------------------------------------------------------------------------------------|---------------------------|---------------------------|
| Customer order number                                                                               | Auftragsnummer des Kunden | 34884                     |
| E+H sales order number                                                                              | E+H Auftragsnummer        | 3019367181000010          |
| Internal order number                                                                               | Interne Auftragsnummer    | 3003840583/0010           |
| Ambient temperature                                                                                 | Umgebungs-Temperatur      | 22.2 °C (± 1 °C)          |
| Ambient humidity                                                                                    | Umgebungs-Luftfeuchte     | 27.9 %rel.F (± 10 %rel.F) |
| Ambient pressure                                                                                    | Umgebungs-Luftdruck       | 980.8 mbar (± 0.2 mbar)   |
| Calibrated according to fix point method IEC 60770. Prüfung nach Grenzpunktmethode gemäß IEC 60770. |                           |                           |

#### Measuring results / Messergebnisse

| Calibration point | Nominal value (p <sub>ref</sub> ) | Measured value (digital readout) | Deviation (digital)  | Nominal value (I <sub>0,ref</sub> calculated) | Current output (analog)       | Rel. deviation (analog)  | Calibration orientation |
|-------------------|-----------------------------------|----------------------------------|----------------------|-----------------------------------------------|-------------------------------|--------------------------|-------------------------|
| Kalibrierpunkt    | Sollwert (p <sub>Ref</sub> )      | Istwert (Digitaler Wert)         | Abweichung (digital) | Sollwert (I <sub>0,ref</sub> berechnet)       | Istwert Stromausgang (analog) | Rel. Abweichung (analog) | Kalibrierlage           |
| %                 | inH <sub>2</sub> O                | inH <sub>2</sub> O               | % of Span            | µA                                            | mA                            | %                        |                         |
| 0                 | 0.00000                           | 0.00040                          | 0.00010              | 4.00000                                       | 3.99994                       | -0.00036                 |                         |
| 51                | 202.402                           | 202.394                          | -0.00197             | 12.09608                                      | 12.09430                      | -0.01115                 |                         |
| 99                | 397.588                           | 397.588                          | -0.00055             | 19.90352                                      | 19.90399                      | 0.00295                  |                         |



Calibration carried out in output mode linear.  
Kalibration erfolgte im Ausgangsmodus linear.

We confirm that all tests, according to the Quality Plan (QP), have been performed successfully.  
At the time of verification, the measuring points of the device indicated above were in compliance to the published valid technical specification (TI).

TI 431P

Measuring point in % of adjusted measuring range/  
Messpunkt in % vom eingestellten Messbereich

Wir bestätigen, dass alle Tests aus dem Qualitätsplan (QP) erfolgreich durchgeführt wurden.  
Das Gerät entspricht zum Zeitpunkt der Prüfung an den aufgeführten Messpunkten den gültigen technischen Spezifikationen (TI).

This document was generated electronically and is valid without signature.

Dieses Dokument wurde elektronisch erzeugt und ist ohne Unterschrift gültig.

**Endress+Hauser**   
People for Process Automation

Date of inspection/ Prüfdatum 26. Nov 2018


11089204/2/0002797-G

- End of document -  
- Ende des Dokuments -

## Hazardous location

Class I, Div. 1, Groups A, B, C, D  
Class I, Zone 0  
AEx ia IIC

## Non hazardous location

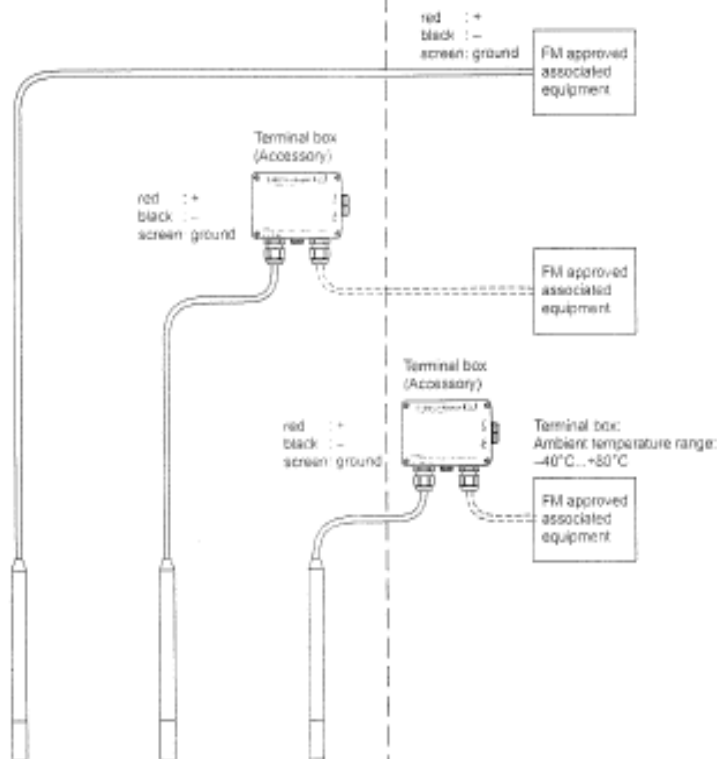


### Sensor

| Temperature class | Ambient temperature range                               |
|-------------------|---------------------------------------------------------|
| T4                | $-10^{\circ}\text{C} \leq T_a \leq +70^{\circ}\text{C}$ |
| T5                | $-10^{\circ}\text{C} \leq T_a \leq +55^{\circ}\text{C}$ |
| T6                | $-10^{\circ}\text{C} \leq T_a \leq +40^{\circ}\text{C}$ |

### Terminal box

| Temperature class | Ambient temperature range                               |
|-------------------|---------------------------------------------------------|
| T6                | $-40^{\circ}\text{C} \leq T_a \leq +80^{\circ}\text{C}$ |

### Terminal box (Accessory):

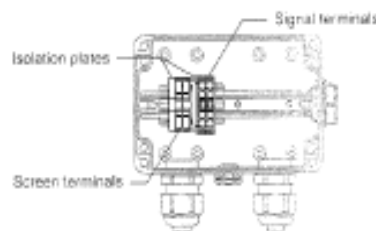

Intrinsically safe (entity), Class I, Div. 1, Groups A, B, C, D or Zone 0, IIC Hazardous Location Installations

1. FM approved apparatus must be installed in accordance with manufacturer instructions.
2. Control room equipment must not use or generate over 250 V.
3. The installation must be in accordance with the National Electric Code ANSI / NFPA 70 and ANSI / ISA-RP 12.08.01.
4. Sensor entity parameters:  $V_{max} = 30\text{ V DC}$ ,  $I_{max} = 133\text{ mA}$ ,  $P_{max} = 1\text{ W}$ . CI and LI per following table:

| Length of sensor cable | CI<br>(10.3 nF + 180 pF/m) | LI<br>(1 $\mu\text{H}/\text{m}$ ) |
|------------------------|----------------------------|-----------------------------------|
| 5 m                    | 11.3 nF                    | 5 $\mu\text{H}$                   |
| 10 m                   | 12.2 nF                    | 10 $\mu\text{H}$                  |
| 20 m                   | 14.0 nF                    | 20 $\mu\text{H}$                  |
| 30 m                   | 15.8 nF                    | 30 $\mu\text{H}$                  |
| 50 m                   | 19.4 nF                    | 50 $\mu\text{H}$                  |
| 100 m                  | 28.4 nF                    | 100 $\mu\text{H}$                 |
| 200 m                  | 48.4 nF                    | 200 $\mu\text{H}$                 |
| 300 m                  | 64.4 nF                    | 300 $\mu\text{H}$                 |

5. FM approved associated equipment must meet following conditions:  
 $V_{oc}$  or  $V_t \leq V_{max}$ ;  $I_{sc}$  or  $I_o \leq I_{max}$ ;  $P_o \leq P_{max}$ ;  
 $C_a \geq C_i + C_{cable}$ ;  $L_a \geq L_i + L_{cable}$ .  
Install associated equipment in accordance with the manufacturer instructions.
6. Use supply wires suitable for 5°C above surrounding ambient.
7. Avoid friction and impact sparks. Anchor sensor if necessary, secure against swinging.
8. WARNING: Avoid electrostatic charging of plastic surfaces. Do not rub. Do not use in media or environments which may generate electrostatic charges on plastic surfaces.
9. WARNING: Substitution of components may impair intrinsic safety.
10. Do not remove or move terminal blocks, fastening elements or insulation plates of the terminal box. Do not build in additional components.
11. Connect cable screen to earth ground of the installation.